Industry: Chemical, Power Product: pH/ORP Analyzer

### Introduction

In limestone-gypsum flue gas desulfurization systems, the consumption of a desulfurization agent (lime) is controlled using online pH analyzers. Of great concern in the pH measurement is heavy lime scaling on the pH electrode. To ensure accurate measurements, frequent cleaning of the electrodes with acid is required, adding to both maintenance workload and cost. The EXA AUTO CLEAN chemical cleaning system automates the acid cleaning process, which not only saves both time and expense but also ensures precise pH measurement over long periods.

# **Expected Benefits**

- Improves the efficiency of a limestone-gypsum flue gas desulfurization system
- Ensures stable, continuous pH measurement
- Reduces operating costs
- Eliminates manual cleaning

# **Process Overview**

The limestone-gypsum flue gas desulfurization consists of two processes: absorption and oxidation. Absorption process


Reaction formula;  $Ca(OH)_2 + CO_2 -> CaCO_3 + H_2O_1 + 2CO_2 + 1/2H_2O_2 -> 2CaSO_3 \cdot 1/2H_2O_3 + CO_2 + 1/2H_2O_3 -> 2CaSO_3 \cdot 1/2H_2O_3 + CO_2 + 1/2H_2O_3 + 1$ 

In this process, it is important to promote the reaction of calcium (Ca) and to achieve a target desulfurization rate. The absorption rate is affected by the pH, concentration, and temperature of liquid and the liquid/gas ratio. When the pH of the absorbing solution is below 5, calcium hydrogen sulfite  $(Ca(HSO_3)_2)$  is generated.  $Ca(HSO_3)_2$  is converted into sulfur dioxide  $(SO_2)$  in a reversible reaction, thereby reducing the desulfurization rate. When the pH of the absorbing solution is 7 or higher, carbon dioxide  $(CO_2)$  in the flue gas reacts with calcium (Ca) to produce calcium carbonate  $(CaCO_3)$ . This increases lime consumption. Since the pH has an influence on the subsequent oxidation process, the pH of the absorbing solution should be kept to between 5 and 6.

#### Oxidation process

Reaction formula:  $CaSO_3 \cdot 1/2H_2O + 1/2O_2 + Aq -> CaSO_4 \cdot 1/2H_2O + Aq$ 

In this process, calcium sulfite ( $CaSO_3 \cdot 1/2H_2O$ ) generated in the absorption process is oxidized with air to calcium sulfate ( $CaSO_4$ ) under a pressure of approximately 500 kPa and a temperature of 50 to 80 °C. The pH of the absorbing solution in the absorber is approximately 6. It should be kept at around 4 by adding acid from the cooling tower.

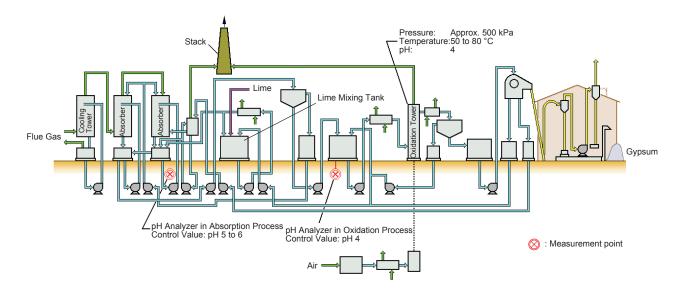





### Solution Details


#### **Field Data**

Deposits of crystalline substances (e.g., CaCO<sub>3</sub>) on electrodes in limestone-gypsum flue gas desulfurization systems decrease the accuracy of pH measurements. The cleaning of the electrodes and the reduction of maintenance time and cost are key points to consider when selecting a pH analyzer for the system.

	pH System with Chemical Cleaning	General pH Analyzer
Cleaning	"Automatic acid cleaning: 2 or 3 times/day, user programmable	"Manual acid cleaning: once/day"
	Manual acid cleaning: approx. monthly"	
Calibration	Manual calibration: weekly	"Manual 2-point calibration: weekly"
Other maintenance	Replenishment of chemical tank: approx. every 2 months	_

Acid cleaning is done with a 4% hydrochloric acid solution

# Measurement System




EXA AUTO CLEAN chemical cleaning system


- 1: PH8HS3 holder
- 2: PH8SM3 operating unit

EXA PH 4-wire pH measurement system

- 3: PH400G 4-wire pH converter
- 4: PH8EFP KCI refillable pH detector


# **Operation Outline**





Sequence Operation
[Measurement]
Measurement takes place when cleaning command is not issued or when measurement command is issued.

Cleaning Status



### [Cleaning]

The pH detector is pulled out of the solution and housed in the cleaning chamber where chemical cleaning takes place. After cleaning, the system moves to measurement mode in accordance with the programmed sequence.

### **Utilities**

Power supply: 100 V AC, 50/60 Hz
Power consumption: approx. 60 VA
Air source: pressure: 300 to 950 kPa

Maximum consumption: approx. 20 L/min

Chemical cleaning solution consumption: approx. 100 mL

Tank effective capacity: approx. 17 L

### **Notes**

- An organic solvent cannot be used for cleaning.
- Deterioration of materials in chemical solution piping and air piping When the system is installed in a location where it is exposed to direct sunlight, the polyethylene resin piping will last approximately one year. (It is recommended that fluoro resin piping be used.)