

General Specifications

Model TDLS8100
Probe type
Tunable Diode Laser Spectrometer

GS 11Y01D02-01EN

Overview

Yokogawa's TDLS™8100 is a laser gas analyzer that measures the concentration of various gases (O₂, CO, CH₄, NH₃, HCl and many more NIR absorbing gases), in various processes such as petrochemical, power generation.

Since it can be inserted directly into duct, the sampling equipment is not required and installation cost and maintenance cost can be reduced. Moreover, it is possible to measure with high accuracy compared to other process analyzers because the measurement is rarely affected by interference of other components in high-speed measurement.

Also, in the conventional laser gas analyzer TDLS™8000, it was necessary to open the installation flange at both ends of the duct, but TDLS™8100 only needs to be done on one side, and if a gas sampling probe is already installed in the existing process, it is possible to replace the gas sampling equipment. If a gas sampling probe is already installed in the existing process, it is easily possible to replace with TDLS8100.



TDLS8100 Probe type
Tunable Diode Laser Spectrometer

Features

• SIL2, TruePeak™ Direct Absorption Spectroscopy combined with smart laser technology

- By calculating the area of the absorbance peak the measurement is not affected by changes of the peak shape due to background gases.
- Fully field repairable
- Continuous diagnostics and 50 days of data storage
- Laser module is replaceable on site without any calibration or adjustment
- Internal reference cell in the laser module ensures peak locking during trace measurement (for O₂ and CO only)
- Laser and Detector modules are sealed to protect them against ingress.
- On board diagnostics and low TCO^(*1) (no moving parts, high MTTF^(*2) for components)
- IEC61508 SIL designed & approved, SIL 2 capability for single analyzer use, SIL 3 capability for dual analyzer use

• Intuitive touchscreen HMI

- Large HMI provides easy operation and control of up to 4 analyzers (TDLS8000 and TDLS8100) at the same time
- A standard mini display enables easy optical alignment

• HART and Modbus TCP communications standard

• 8-stage auto-gain adapts to difficult applications

- Auto-gain enables wide signal ranges against dynamic variation of transmission.

• Compact design for one-man installation without sacrificing ruggedness

- FM (US, Canada), IECEx, ATEX/UKEX hazardous area, Korea, NEPSI, Japan approvals based on Explosionproof/flame proof.

• In-situ analysis and fast response (2 seconds, 1 second (optional))

• Process temperatures up to 600 °C, process pressures up to 500 kPa abs., and process gas flow velocity 1 m/s or more.

Note: Maximum process temperatures and pressures will vary by application.

• 10 different languages display options

YH8000 offers easy touch screen operation and simple menu structure in 10 languages.

Typical gases measured include:

- Oxygen in process applications.
Process temperatures can be as high as 600°C, and process pressures can be as high as 500kPa abs. Measurement span is typically between 1% and 25% oxygen.
- Carbon monoxide in process applications.
Process temperatures can be as high as 600°C.

Other applications and gas measurements are possible with the TDLS8100.

Please fill out the Application Data Sheet at the end of this document and send to Yokogawa.

*1: Total Cost of Ownership

*2: Mean Time To Failure


TDLS, TruePeak are trademarks or registered trademarks of Yokogawa Electric Corporation.

All other company and product names mentioned in this document are trademarks or registered trademarks of their respective companies.


Please select appropriate equipment in accordance with the laws and regulations of the relevant country/region, when it is used in a location where explosive atmospheres may be present.

■ System configuration


Standard System Configuration

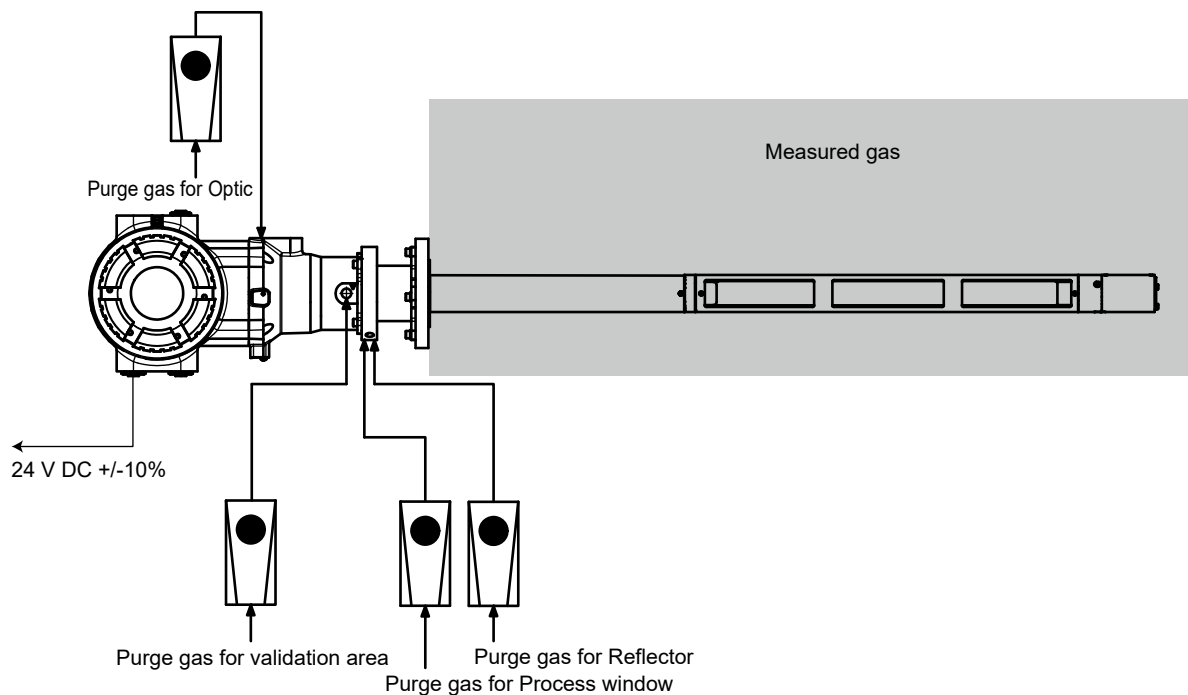

System Configuration with YH8000 HMI Unit and Validation gas line

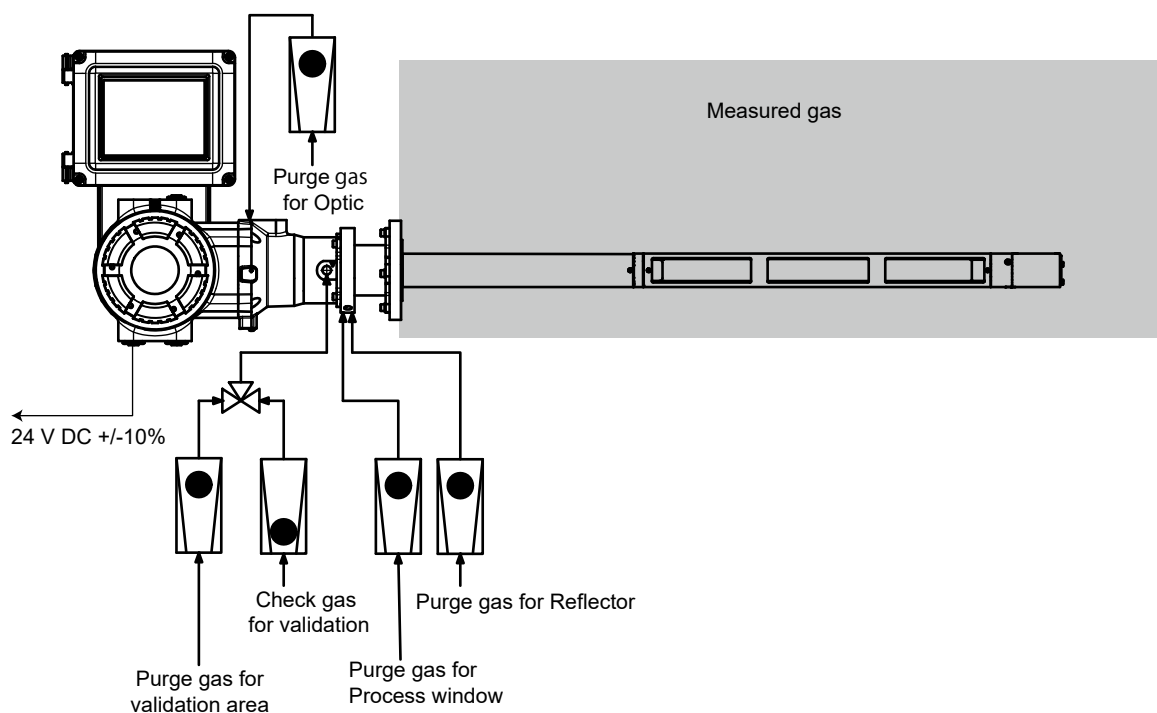

Multi Analyzer Configuration with Remote HMI

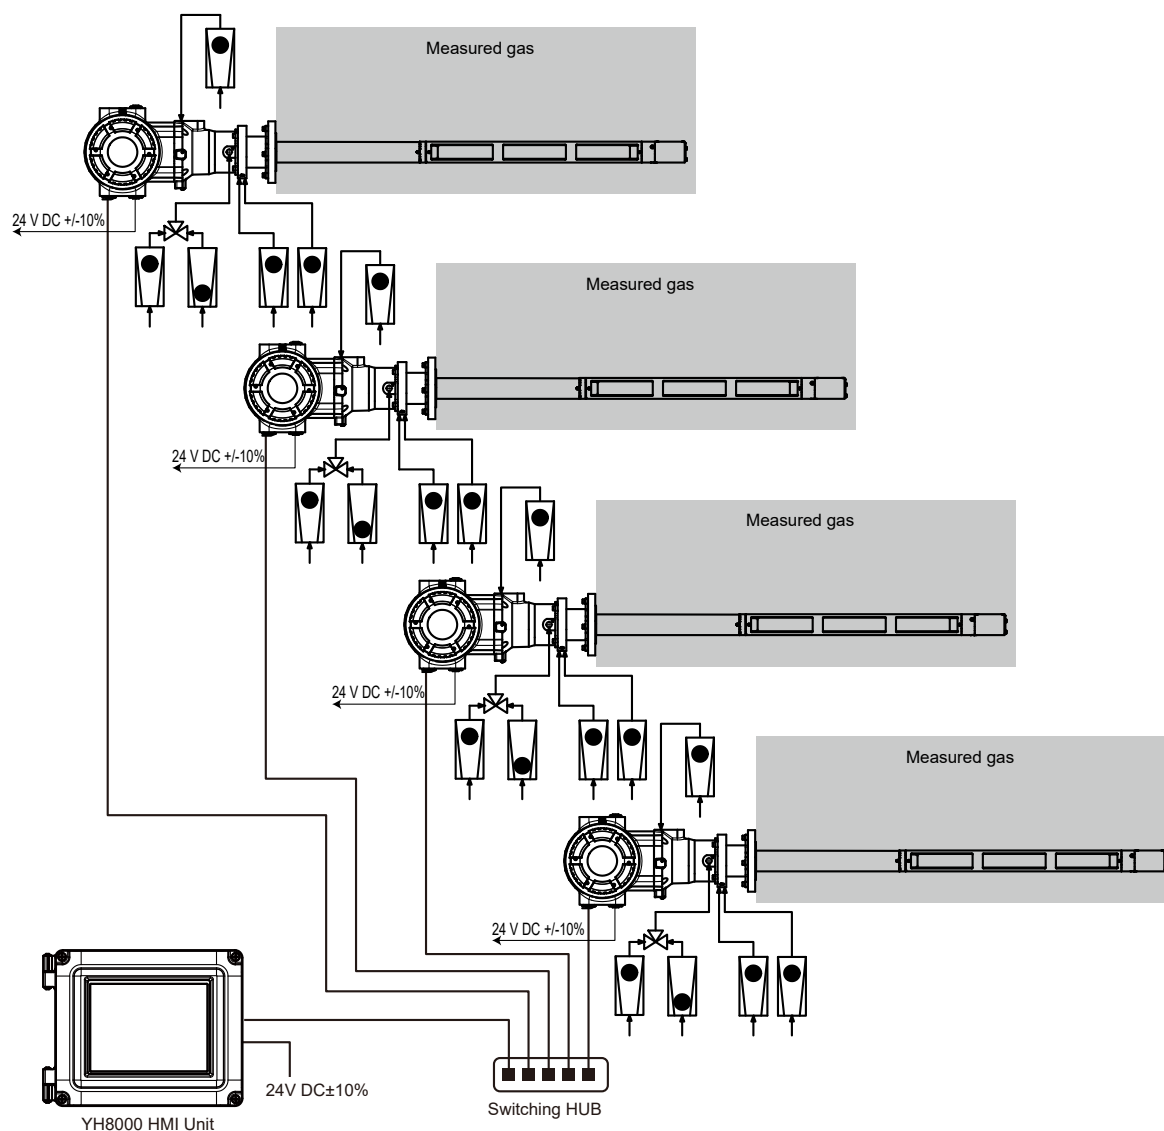

Note: If power supply is 100 to 240 V AC, purchase the Universal Power Supply, separately.
 If four multi analyzer configuration with remote HMI is made, five universal power supplies including YH8000 are needed.

■ STANDARD SPECIFICATIONS

● TDLS8100 Probe type Tunable Diode Laser Spectrometer

Measurement object:

O₂, CO, CO or CH₄, NH₃, HCl
concentration in combustion exhaust
gas and process gas If other gas
measurements are required, consult with
Yokogawa

Measurement system:

Tunable diode laser spectroscopy
Light source; Near-infrared tunable diode laser

Measured components and ranges:

Measured component	Min. range	Max. range
O ₂	0-1%	0-25% (*2)
CO (*1)	0-200 ppm	0-10,000 ppm
CH ₄ (*1)	0-5%	
NH ₃	0-30 ppm	0-5000 ppm
HCl	0-50 ppm	0-5000 ppm

*1: Please consult with Yokogawa if CO and CH₄
ingredient coexists.

*2: In the case of explosionproof type, oxygen
concentration shall not exceed that found in
normal air, typically 21%.

Safety and EMC conformity standards:

Safety conformity standards:

CE, UKCA EN61010-1, EN61010-2-030
UL UL61010-1, UL 61010-2-030
CSA CAN/CSA-C22.2 No.61010-1, CAN/
CSA-C22.2 No.61010-2-030
GB GB30439 Part 1

Installation altitude: 2000 m or less

Installation category:

I (Anticipated transient overvoltage 330V)

Measuring category: O (Other)

Pollution degree: 2, Indoor/Outdoor use

Note: Installation category, called overvoltage category,
specifies impulse withstand voltage. Pollution
degree indicates the degree of existence of solid,
liquid, gas or other inclusions which may reduce
dielectric strength.

EMC conformity standards:

CE, UKCA EN55011 Class A Group 1
EN61326-1 Class A Table 2 (For use in
industrial location), EN61326-2-3
RCM EN55011 Class A Group 1
KC KN11 Class A Group 1, KN61000-6-2
(Korea Electromagnetic Conformity)

Laser classification:

CSA E60825-1:15,
GB7247.1-2012, FDA 21 CFR part 1040.10,
Class 1 laser product

SIL Certification:

The TDLS8100 except digital output (2 points),
digital input (2 points), valve control output (2
points), and digital communications (HART,
Modbus/TCP) are certified in compliance with
the following standard.

IEC 61508:
Functional safety of Electrical/electronic/
programmable electronic related systems
SIL 2 capability for single analyzer use,
SIL 3 capability for dual analyzer use.

RoHS conformity standards: EN IEC 63000:2018*

*: For only TDLS8100-G1, -G2, -S1

Information of the WEEE Directive

This product is purposely designed to be used
in a large scale fixed installations only and,
therefore, is out of scope of the WEEE Directive.
The WEEE Directive does not apply.

The WEEE Directive is only valid in the EU and
UK.

Display: 128 x 64 dots LCD; On Sensor Control Unit
Status LEDs; (Green: Power, Orange: DO,
Red: Fault)

Display items:

Gas concentration, Transmission,
Process gas temperature (AI), Process
gas pressure (AI), System status,
Alarm information, System information
(Product serial no., Laser detector
module serial no., Output signal, IP
address, HART address, Optical path
length, Analyzer internal temperature)

Analog output:

2 points, 4 to 20 mA DC (Isolated from
the power supply and ground, Max. load
sistance 550 Ω)

Output types; Gas concentration, Transmission,
Process gas temperature, Process
gas pressure

Output range; 3.0 to 21.6 mA DC

Digital communications:

HART; On analog output signal 1 (AO-1)

Load resistance;
250 to 550 Ω (Include cable resistance)

Ethernet; RJ-45 connector

Protocol; Modbus/TCP

Communication speed; 100 Mbps

Digital output: 2 points, contact rating 24
V DC, 1A

DO;

Function: Activate during Warning / Calibration
/ Validation / Warm up / Maintenance
conditions

Contact Specification: Relay contact output
(Isolated from the power supply and
ground), C-contact (NC/NO/COM)

Fault;

Function: Activate during Fault condition or when
the system power is off

Contact Specification: Relay contact output
(Isolated from the power supply and
ground), A-contact (NC/COM)

Valve control output: 2 points

Function; Activate calibration or validation solenoid
valves for zero, span or validation gas.

Output signal; 24V DC, 500 mA Max. per terminal

Alarm:

Warning; Gas concentration low, Gas concentration
high, Transmission low, Process pressure
low, Process pressure high, Process
temperature low, Process temperature
high, Validation required, Validation
failure, Zero calibration error, Span
calibration error, External alarm, Detector
signal high, Absorption too high

Fault; Laser module temperature low, Laser module temperature high, Laser temperature low, Laser temperature high, Peak center out of range, Reference peak height low, Transmission lost, Reference transmission low, Reference peak height high, Laser unit failure, Laser module error, File access error, E2PROM access error

Digital input: 2 points

Function; External Alarm/Calibration start/Validation start/Stream switch (Valve control)

Contact specification; Zero voltage contact input (Isolated from the power supply and ground)

Input signal; Open signal: 100 kΩ or more, Close signal: 200 Ω or less

Analog input: 2 points

Signal type; 4 to 20 mA DC (Isolated from the power supply and Ground), with selectable powered/unpowered function

Input signal range; 2.4 to 21.6 mA DC

Input types; Process gas temperature, Process gas pressure

Transmitter power supply; 15 V DC or higher (at 20 mA DC) 26 V DC or less (at 0 mA DC)

Self-diagnostics:

Laser detector Unit temperature, Laser temperature, Detector signal level, Memory read/write function, Peak locking condition

Calibration:

Calibration method; Zero/Span calibration

Calibration mode; Manual, Semi-Auto (YH8000/HART)

Validation:

Validation method; Up to 2 points

Validation mode; Manual, Auto (Time initiated, Remote initiate (DI/Modbus)), Semi-Auto (YH8000/HART)

Power supply: 24V DC +/-10%

Power consumption:

Max. 20W; TDLS8100 only

Max. 60W; TDLS8100 with YH8000 and 2 solenoid valves

Protection degree: IP66, Type 4X

Material: Case; Aluminum alloy

Wetted materials: 316 SS(eq.), BK-7 glass, Teflon encapsulated FKM, ASE wool

Paint color: Mint green (RAL 190 30 15 or equivalent)

Weight (approx.):

Probe part;

0.7 m 2.7 kg, 1 m 4.3 kg, 1.5 m 7.0 kg, 2 m 9.8 kg

Analyzer part;

explosion proof 15.7 kg, general purpose 14.8 kg (Not include flange)

Process gas condition:

Process gas temperature; Max. 600°C, Application dependent

Process gas pressure; Max. 500 kPa abs., Min. 90 kPa abs., Application dependent

Process gas velocity; over 1m/s (recommendation over 5 m/s)

Dust in process gas; When the process dust load is high, please consult with Yokogawa.

Note: When using TDLS8100 as CE/UKCA marking compliance product, it has following limitation. General purpose model (-G1, -G2): The upper limit of the measurement gas pressure is 50kPa in gauge pressure. ATEX/UKEX model (-S1): The upper limit of the measurement gas pressure is 500kPa abs. The unstable gas defined by following cannot be measured. An unstable gas in this context is a gas liable to transform itself spontaneously, producing a sudden pressure increase. Such transformation as an example can result from a relatively small variation of an operating parameter (e.g. pressure, temperature, presence of catalyzing material) in a confined volume. This includes gases that are classified as chemically unstable gases according to CLP Regulation (EC) No 1272/2008 as amended. Typical examples of unstable gases: acetylene (UN 1001), methyl acetylene (UN 1060), vinylfluoride (UN 1860), ozone and dinitrogen oxide (UN 1067). For further examples, see Table 35.1 of the UN Manual of Tests and Criteria.

Warm-up time: 5 min.

Installation condition:

Ambient operating temperature; -20 to 55°C

Storage temperature; -30 to 70°C

Humidity; 0 to 95%RH at 40°C (Non-condensing)

Mounting flange type; ASME B16.5, DIN, JIS

Cable entries; 1/2NPT or M20x1.5mm, one hole. 3/4NPT or M25x1.5mm, three holes

Purge gas connections;

1/4NPT or Rc1/4

If other gas connections are required, please consult with Yokogawa.

Purge gas; Theoretically, instrument air could be used as a purge gas for all the below applications except for oxygen measurement. Choosing between using nitrogen or instrument air or purge gas will ultimately depend upon further application details and the desired precision of the measurement. All gasses should be clean and dry.

Recommended purge gasses:

O₂ analyzer: N₂ (99.99% or greater, application dependent)

CO, CO or CH₄, NH₃, HCl analyzer: N₂ (99.99% or greater, application dependent) or Instrument air (dew point; less than -20°C/no dust/no oil mist)

Purge gas flow rates;

Optic: 2 to 20L/min (Application dependent) 2 to 20L/min and 100 to 200mL/min (explosionproof)

* Not more than 10 kPa at the inlet for explosionproof

Process window/Reflector:

5 to 30L/min (Application dependent)

Hazardous area classifications:

Division1, Zone1 Explosionproof

TDLS8100-D1 (FM Approval for US)

Division system:

Type pf protection:

Explosion proof; Class I, Division 1, Groups A, B, C, D, T6

Dust-Ignitionproof; Class II/III, Division 1, Groups E, F, G T6

Enclosure rating: Type4X

Applicable standards:

FM Class 3600: 2018,
FM Class 3615: 2018,
FM Class 3616: 2011,
FM Class 3810: 2018,
NEMA 250: 2014,
ANSI/ISA-12.27.01: 2011

Zone system:**Type of protection:**

Class I, Zone 1, AEx db [op is Ga] IIC T6 Gb
Zone 21, AEx tb [op is Da] IIIC T85°C Db

Enclosure rating: IP66**Applicable standards:**

ANSI/UL 60079-0:2013
ANSI/UL 60079-1: 2015,
ANSI/UL 60079-28:2017,
ANSI/UL 60079-31: 2015,
ANSI/IEC 60529:2004,
ANSI/ISA-12.27.01: 2011

TDLS8100-C1 (FM Approval for Canada)**Type of protection:**

Ex db [op is Ga] IIC T6 Gb
Ex tb [op is Da] IIIC T85°C Db

Enclosure rating: IP66, Type4X**Applicable standards:**

CSA C22.2 No.94.2-15:2015,
CAN/CSA C22.2 No.60079-0: 2015,
CAN/CSA C22.2 No.60079-1: 2016,
CAN/CSA C22.2 No.60079-28: 2016,
CAN/CSA C22.2 No.60079-31: 2015,
CAN/CSA C22.2 No.60529: 2016,
CAN/CSA-C22.2 No. 61010-1-12:2012,
CAN/CSA-C22.2 No. 61010-2-030-12:2016,
ANSI/ISA-12.27.01: 2011

TDLS8100-E1 (IECEx)**Type of protection:**

Ex db [op is Ga] IIC T6 Gb
Ex tb [op is Da] IIIC T85°C Db

Enclosure rating:

IP66 (In Accordance with IEC 60529)

Applicable standards:

IEC 60079-0:2017,
IEC 60079-1:2014,
IEC 60079-28:2015,
IEC 60079-31:2013

TDLS8100-S1 (ATEX/UKEX)**Type of protection:**

II 2(1) G Ex db [op is Ga] IIC T6 Gb
II 2(1) D Ex tb [op is Da] IIIC T85°C Db

Enclosure rating:

IP66 (In Accordance with EN 60529)

Applicable standards:

EN IEC 60079-0:2018
EN 60079-1:2014, EN 60079-28:2015,
EN 60079-31:2014

TDLS8100-K1 (Korea Ex)**Type of protection:**

Ex db IIC T6 Gb
Ex tb IIIC T85°C Db

Enclosure rating: IP66 (In Accordance with IEC 60529)**Applicable standards:**

Notice of Ministry of Labor No. 2021-22
Harmonized with IEC 60079-0: 2017,
IEC 60079-1: 2014,
IEC 60079-31: 2013

TDLS8100-N1 (NEPSI)

Type of protection: Ex db [op is Ga] IIC T6 Gb
Ex tb [op is Da] IIIC T85°C Db

Enclosure rating: IP66

(in accordance with GB/T 4208-2017)

Applicable standards:

GB/T 3836.1-2021
GB/T 3836.2-2021
GB/T 3836.22-2017
GB/T 3836.31-2021

TDLS8100-J1 (Japan Ex)

Type of protection: Ex db [op is Ga] IIC T6 Gb
Ex tb [op is Da] IIIC T85°C Db

Enclosure rating: IP66

(In Accordance with IEC 60529)

Applicable standards:

JNIOH-TR-46-1:2020
JNIOH-TR-46-2:2018
JNIOH-TR-46-9:2018
JNIOH-TR-46-11:2020

PERFORMANCE**Repeatability / Linearity:**

Measured gas		Repeatability	Linearity
O ₂		+/- 1% reading or +/- 0.01 %O ₂ , whichever is greater	+/- 1% F.S.
CO (ppm)		+/- 2% reading or +/- 1 ppm CO, whichever is greater	+/- 1% F.S.
CO or CH ₄	CO	+/- 2% reading or +/- 1 ppm CO, whichever is greater	+/- 2% F.S.
	CH ₄	+/- 4% reading or +/- 0.02% CH ₄ , whichever is greater	+/- 4% F.S.
NH ₃		+/- 2% reading or +/- 1ppm NH ₃ , whichever is greater	+/- 2% F.S.
HCl		+/- 1% reading or +/- 2.5ppm HCl, whichever is greater	+/- 2% F.S.

Measurement conditions: Gas temperature; 25 °C,
Gas pressure; 0.1 MPa,
Optical path length; 1 m

Data Update**Cycle:**

Approx. 2 seconds (Response time may increase for non-standard applications) If less than 2 seconds response is required, please consult with Yokogawa

Influences on the Measurement - Application dependent

A. Temperature: The temperature of the measured gas should be taken into account by the analyzer so that the reading can be corrected on a real time basis. The effect is specific to each different measurement gas.

- If the gas temperature is constant at the desired measurement condition, then a fixed gas temperature may be programmed into the analyzer. This fixed value can be used in real time by the analyzer to provide a temperature-compensated reading.
- If the gas temperature is relatively equal to the ambient temperature, then an integral sensor value may be utilized by the analyzer. This active ambient value is used real time by the analyzer to provide a temperature compensated reading.

- c. If the gas temperature is variable, then an external sensor value may be utilized by the analyzer. This active input value can be used in real time by the analyzer to provide a temperature compensated reading.
- B. Pressure: The pressure of the measured gas must be taken into account by the analyzer so that the reading can be corrected on a real time basis. The effect is specific to each different measurement gas.
 - a. If the gas pressure is constant at the desired measurement condition, then a fixed gas pressure may be programmed to the analyzer. This fixed value can be used in real time by the analyzer to provide a pressure compensated reading.
 - b. If the gas pressure is variable, then an external sensor value may be utilized by the analyzer. This active input value can be used in real time by the analyzer to provide a pressure compensated reading.

● YH8000 HMI Unit

The YH8000 is an HMI designed specifically for the TDLS8000 series. The YH8000 features an easy-to-use touchscreen 7.5 inch color LCD which can be used to display maintenance information, display alarm statuses and records, and set all parameters of the TDLS8100.

The YH8000 can be installed directly on the TDLS8000 series or installed remotely.

An Ethernet connection is used to connect the YH8000 to up to four TDLS8000 series simultaneously via a hub.

Display: Touchscreen 7.5 inch TFT color LCD panel, 640 x 480 (VGA)
 Communication: Ethernet; RJ-45 connector
 Communication speed: 100 Mbps
 Case: Aluminum alloy
 Paint color: Mint green (RAL 190 30 15 or equivalent)
 Protection degree of enclosure: IP65, Type 4X
 Window: Polycarbonate
 Weight: Approx. 4 kg
 Cable gland for Japan Ex: (/JA1, /JA2) Approx. 320 g/pc
 Mounting: Analyzer mount (Front, left-side, right-side) with tilt function, Pipe mount, or Panel mount (Stainless steel)
 Cable Entries: 1/2NPT or M20x1.5 mm, two holes
 Installation conditions:
 Ambient operating temperature: -20 to 55°C
 Storage temperature: -30 to 70°C
 Humidity: 10 to 90%RH at 40°C (Non-condensing)
 Power Supply: 24V DC +/-10%
 Power consumption: Max. 12 W
 Safety, EMC, and RoHS conformity standards:
 Safety conformity standards:
 CE, UKCA EN61010-1
 UL UL61010-1
 CSA CAN/CSA-C22.2 No.61010-1
 GB GB30439 Part 1
 Installation Altitude: 2000 m or less
 Installation category: I
 (Anticipated transient overvoltage 330 V)
 Pollution degree: 2, Indoor/Outdoor use

EMC conformity standards:

CE, UKCA EN55011 Class A Group 1
 EN61326-1 Class A Table 2 (For use in industrial location)

RCM EN55011 Class A Group 1
 KC KN11 Class A Group 1, KN61000-6-2 (Korea Electromagnetic Conformity)

RoHS conformity standards: EN IEC 63000:2018*

*: For only YH8000-G1, -G2, -S2

Information of the WEEE Directive

This product is purposely designed to be used in a large scale fixed installations only and, therefore, is out of scope of the WEEE Directive. The WEEE Directive does not apply. The WEEE Directive is only valid in the EU and UK.

Hazardous area classifications:

Division 2, Zone2: Nonincendive/Type n

YH8000-D2 (FM Approval for US)

Division system

Type of protection: Nonincendive for Class I, Division 2, Groups A, B, C, D, T5

Enclosure rating: Type 4X

Applicable standards: FM Class 3600: 2018
 FM Class 3611: 2018
 FM Class 3810: 2018
 NEMA 250: 2003

Zone system

Type of protection:

Class I, Zone 2, AEx nA ic IIC T5 Gc

Enclosure rating: IP65

Applicable standards: ANSI/UL 60079-0:2019,
 ANSI/UL 60079-11:2013
 ANSI/UL 60079-15:2013
 ANSI/UL 121201:2019
 ANSI/IEC 60529-2004

YH8000-C2 (FM Approval for Canada)

Type of protection: Ex nA ic IIC T5 Gc

Enclosure rating: IP65, Type 4X

Applicable standards:
 CAN/CSA No.94.2-07 (R2012)
 CAN/CSA-C22.2 No.60079-0:19
 CAN/CSA-C22.2 No.60079-11:14
 CAN/CSA-C22.2 No.60079-15:16
 CAN/CSA-C22.2 No.61010-1-12
 CAN/CSA No.60529:05 (R2010)

YH8000-S2 (ATEX)

Type of protection: II 3 G Ex nA ic IIC T5 Gc

Enclosure rating: IP65 (In accordance with EN 60529)

Applicable standards:
 EN IEC 60079-0:2018,
 EN 60079-11: 2012, EN 60079-15: 2010

YH8000-E2 (IECEx)

Type of protection: Ex nA ic IIC T5 Gc

Enclosure rating: IP65 (In accordance with IEC 60529)

Applicable standards: IEC 60079-0: 2017,
 IEC 60079-11: 2011, IEC 60079-15: 2010

YH8000-J2 (Japan Ex)

Type of protection: Ex nA ic IIC T5 Gc

Enclosure rating: IP65 (In accordance with IEC 60529)

Applicable standards: JNIOH-TR-46-1:2020
 JNIOH-TR-46-6:2015
 JNIOH-TR-46-8:2015

YH8000-K2 (Korea Ex)

Type of protection: Ex nA ic IIC T5 Gc
 Enclosure rating: IP65 (In accordance with IEC 60529)
 Applicable standards: Notice of Ministry of LaborNo. 2021-22
 Harmonized with IEC60079-0: 2017, IEC 60079-11: 2011, IEC 60079-15:2010

YH8000-N2 (NEPSI)

Type of protection: Ex ec ic IIC T5 Gc
 Enclosure rating: IP65 (In accordance with GB/T 4208-2017)
 Applicable standards: GB/T 3836.1-2021, GB/T 3836.3-2021, GB/T 3836.4-2021

YH8000-R2 (EAC)

Type of protection: 2Ex nA ic IIC T5 Gc X
 Enclosure rating: IP65 (In accordance with GOST 14254)
 Applicable standards: GOST 31610.0-2014
 GOST 31610.15-2014
 GOST 31610.11-2014

YH8000-U2 (INMETRO)

Type of protection: Ex nA ic IIC T5 Gc
 Enclosure rating: IP65
 Applicable standards: ABNT NBR IEC 60079-0:2020
 ABNT NBR IEC 60079-11:2013
 Versão Corrigida:2017
 ABNT NBR IEC 60079-15:2019

- **Calibration Cell**

Used for off-line calibrations and validations.

Optical Path Length: 500 mm
 Material: 316 SS (eq.), Aluminum, BK-7, FKM
 Part No.: K9777ZA (for O₂, CO), K9777ZK (for NH₃), K9777ZL (for HCl)
 Weight: Approx. 4.6 kg

■ MODEL AND CODES

● TDLS8100 Probe type Tunable Diode Laser Spectrometer (Note)

Model	Suffix Code	Option Code	Description
TDLS8100	Probe type Tunable Diode Laser Spectrometer
Structure	-G1 -G2 -D1 -C1 -E1 -S1 -K1 -N1 -J1	General Purpose, cable entry/piping:NPT General Purpose, cable entry:Metric thread, piping:Rc FM (US) explosionproof, cable entry/piping: NPT FM (Canada) explosionproof, cable entry/piping: NPT IECEX explosionproof, cable entry:Metric thread, piping:Rc ATEX/UKEX explosionproof, cable entry:Metric thread, piping:Rc Korea explosionproof: cable entry:Metric thread, piping: Rc NEPSI explosionproof: cable entry:Metric thread, piping: Rc Japan Ex explosionproof: cable entry:Metric thread, piping: Rc (*6)
Temperature	-L	Standard < 600 degC
Gas Parameter	-X1 -C2 -C3 -C4 -A1 -L1	O ₂ < 600°C, 0-25% (*1) CO ppm <500°C (*2) CO ppm <600°C for combustion (*2) CO ppm <500°C or CH ₄ 0-5% for combustion (*2) NH ₃ up to 0-5,000 ppm <450°C DeNOx HCl 0-50 ppm/0-5,000 ppm <500°C
—	-NN	Always -NN
Probe length	-070 -100 -150 -200	0.7m 1m 1.5m 2m
Probe material	-S	316SS
Flange	-U2 -U3 -U4 -D5 -D8 -J5 -J8	ANSI CLASS150-2-RF(Eq.) ANSI CLASS150-3-RF(Eq.) ANSI CLASS150-4-RF(Eq.) DIN PN16-DN50-D(Eq.) DIN PN16-DN80-D(Eq.) JIS 10K-50-FF(Eq.) JIS 10K-80-FF(Eq.)
I/O interface	-A1	Analog with HART + Modbus Ethernet
SI Unit	-J -N	Only SI unit SI unit or non SI unit (*3)
—	-N	Always -N
Option		/RX /RC /SCT /SIL /JA1 /JB1 /JB2 /JB3	Reference Cell for O ₂ (*4) Reference Cell for CO (*5) Stainless Steel Tag Plate With IEC61508 SIL2 (SC3) Cable gland for Japan Ex (Cable O.D. 8-12mm, G1/2) 1pc, for local HMI Cable gland for Japan Ex (Cable O.D. 10-16mm, G3/4) 1 pcs Cable gland for Japan Ex (Cable O.D. 10-16mm, G3/4) 2 pcs Cable gland for Japan Ex (Cable O.D. 10-16mm, G3/4) 3 pcs

*1: When the process gas pressure is out of 90 to 130 kPa (abs.), or the process gas contains CO₂ ≥ 40 % or H₂ ≥ 20 % as coexisting gas components, please contact YOKOGAWA.

*2: When CO and CH₄ ingredient coexist, please contact YOKOGAWA.


*3: Enable only to an end user located outside of Japan

*4: The Option "/RX" can be used when Gas Parameter "-X1" is selected.

*5: The Option "/RC" can be used when Gas Parameter "-C2", "-C3" or "-C4" are selected. When both "-C3" or "-C4" of the Gas Parameter is selected, "/RC" must be specified.

*6: For Japan Ex model (TDLS8100-J1), specified cable glands shall be attached to each cable entry for wiring. Select one cable gland out of three types: (/JB1, /JB2, or /JB3). If you need, specify (/JA1) as well. For detailed information, refer to Japanese General Specifications.

(Note) When arranging TDLS8100, please refer to the following matrix and specify "probe, indicator direction" with the number of [].

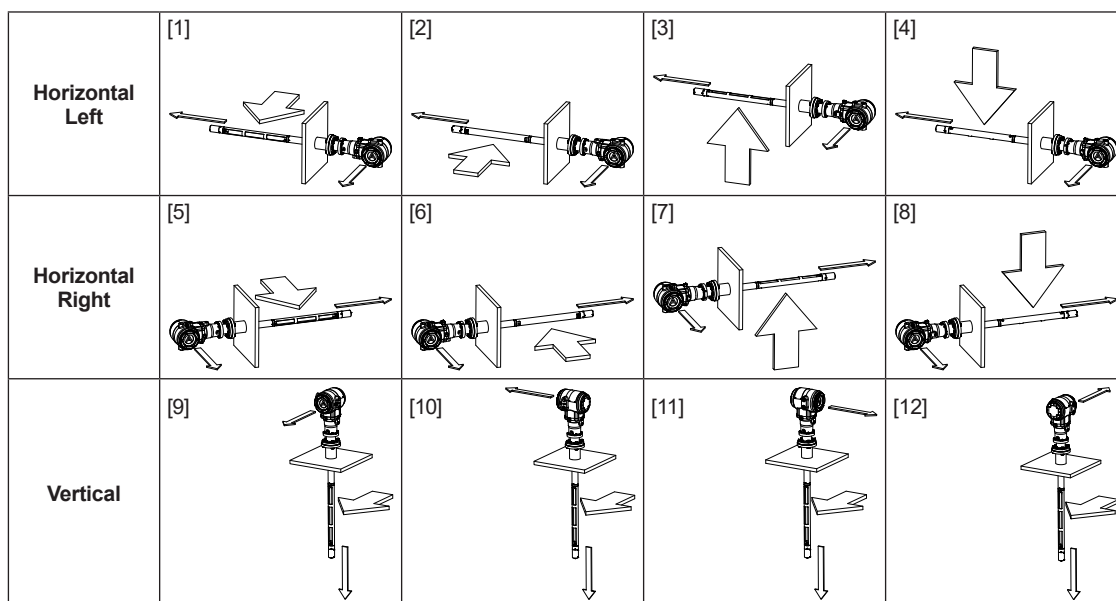

vertical upwards is not possible

● YH8000 HMI Unit

Model	Suffix Code	Option Code	Description
YH8000	HMI Unit
Type	-G1 -G2 -GR -D2 -C2 -S2 -E2 -J2 -K2 -N2 -R2 -U2	General Purpose, NPT thread for cable entry General Purpose, Metric thread for cable entry EAC General Purpose, Metric thread for cable entry FM (US) Class I Div 2, Zone2, NPT thread for cable entry FM (Canada) Class I Zone2, NPT thread for cable entry ATEX Type of protection "n", Metric thread for cable entry (*3) IECEx Type of protection "n", Metric thread for cable entry Japan Ex / Zone 2, Metric thread for cable entry (*2) Korea Ex Type of protection "n", Metric thread for cable entry NEPSI Increased safety "ec", Metric thread for cable entry EAC Type of protection "n", Metric thread for cable entry INMETRO Type of protection "n", Metric thread for cable entry
Language	-E	English and 9 languages (*1)
—	-N	Always -N
Option	/M /P /W /S /C /SCT /JA1 /JA2	Mounting kit for TDLS8000 series Pipe mount Wall mount Sun Shield Local HMI connection cable: 3m Stainless Steel Tag Plate Cable gland for Japan Ex (Cable O.D. 8-12mm, G1/2), 1 pc(*2) Cable gland for Japan Ex (Cable O.D. 8-12mm, G1/2), 2 pc(*2)

*1: These languages are message languages on the display.

One analyzer has English and 9 languages.

All languages are as follows; English, German, French, Spanish, Portuguese, Russian, Hungarian, Korean, Chinese and Japanese.

*2: For Japan Ex/Zone 2 certified model (YH8000-J2), specified cable glands shall be attached to each cable entry for wiring. For detailed information, refer to Japanese General Specifications (GS 11Y01D01-01JA).


The Option "/JA1" and "/JA2" can be used only when Japan Ex/Zone 2 certified model (YH8000-J2) is selected.

If "/JA1" or "JA2" is necessary for other model, please contact Yokogawa.

*3: This model is available for UKCA.


EXTERNAL DIMENSIONS

TDLS8100 Probe type Tunable Diode Laser Spectrometer

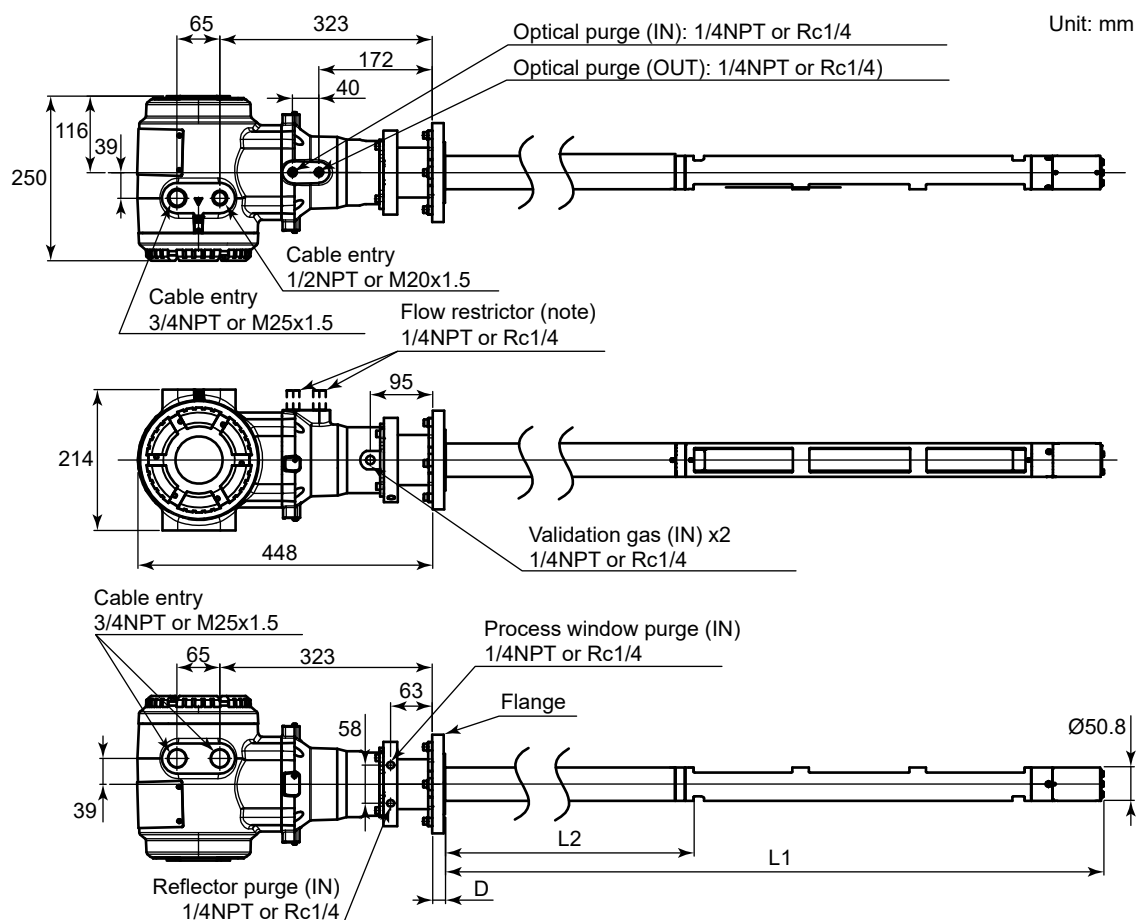

Flange	A	B	C	D
ANSI Class150-2-RF	150	120.7	4-Ø19	20
ANSI Class150-3-RF	190	152.4	4-Ø19	24
ANSI Class150-4-RF	230	190.5	8-Ø19	24
DIN PN16-DN50-D	165	125	4-Ø18	20
DIN PN16-DN80-D	200	160	8-Ø18	20
JIS 10K-50-FF	155	120	4-Ø19	16
JIS 10K-80-FF	185	150	8-Ø19	18

L1	700	1000	1500	2000
L2	78	378	878	1378


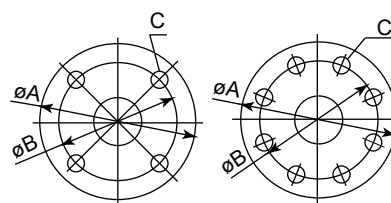


Flange

(note) The flow restrictors are attached
in the case of type -C1, -D1, -E1, -S1, -K1, -N1, -J1

- Maintenance space

Unit: mm

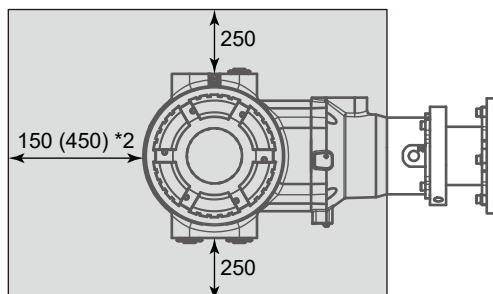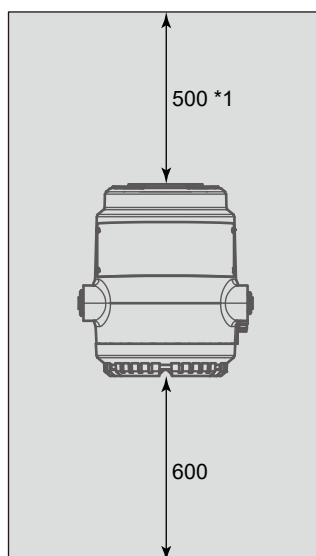


*1: When installing YH8000 on TDLS8100 with /M, it is necessary to secure this space.


*2: When connecting the calibration cell, it is necessary to secure this space. If install or uninstall of probe, need the additional space depend on probe length.

• Flowcell type (reference)


For applications where the TDLS8000 or TDLS8100 could not be installed or inserted due to the process size, etc., a sampling system can be constructed by replacing the probe part of the TDLS8100 with a flow cell part. Please contact Yokogawa.

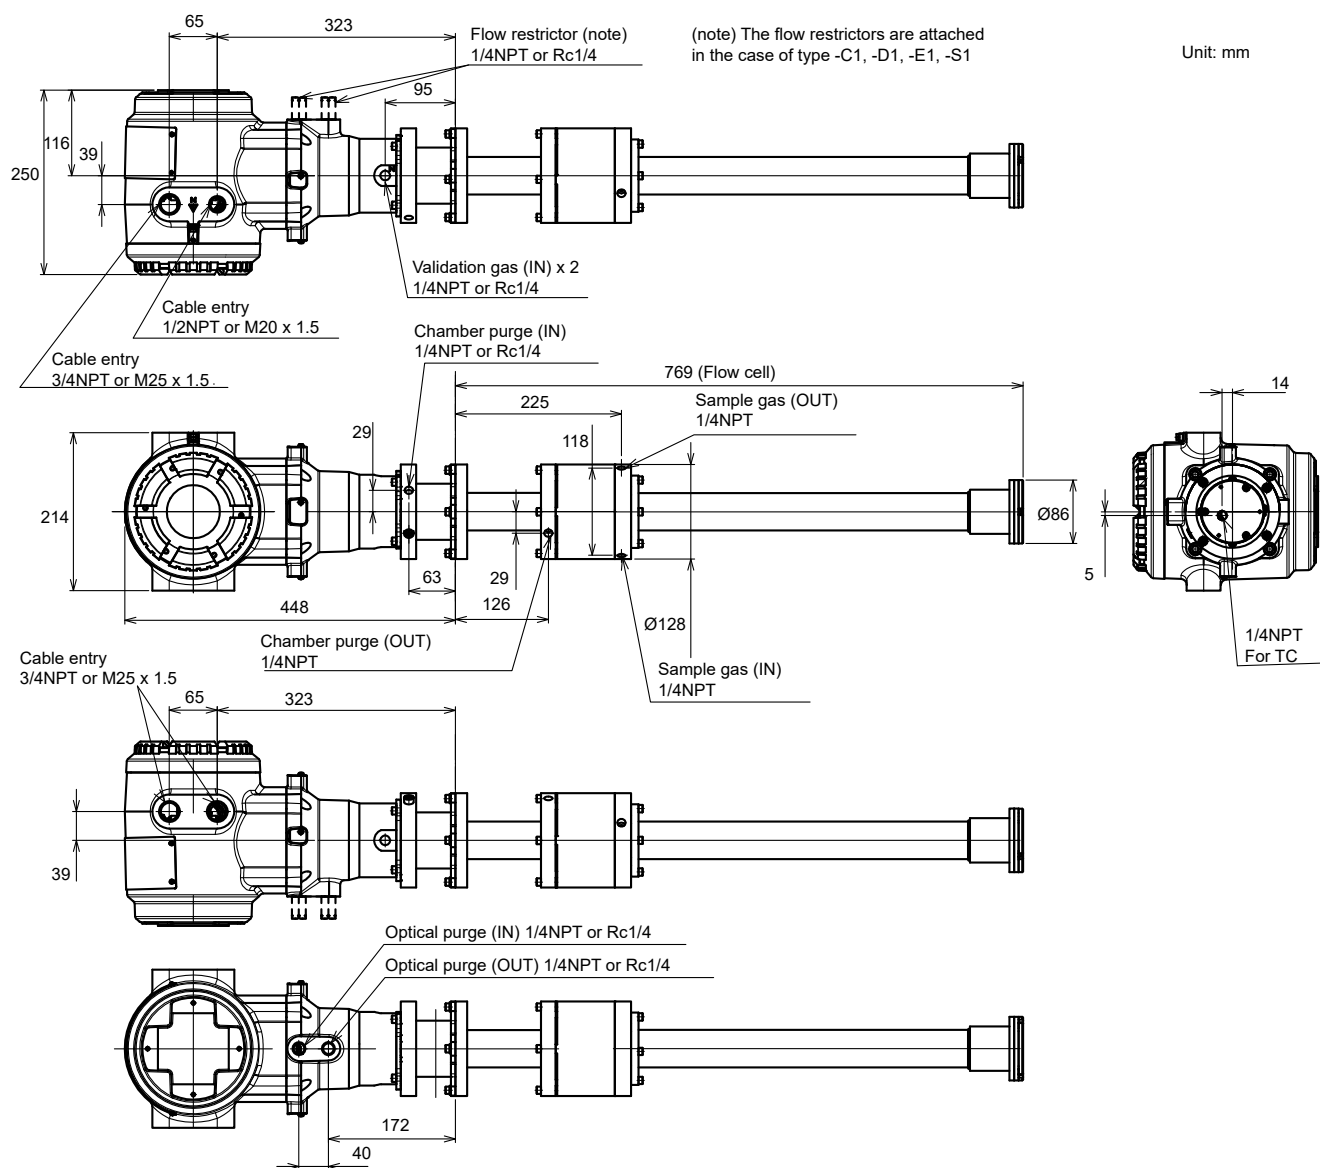




■ YH8000 HMI Unit

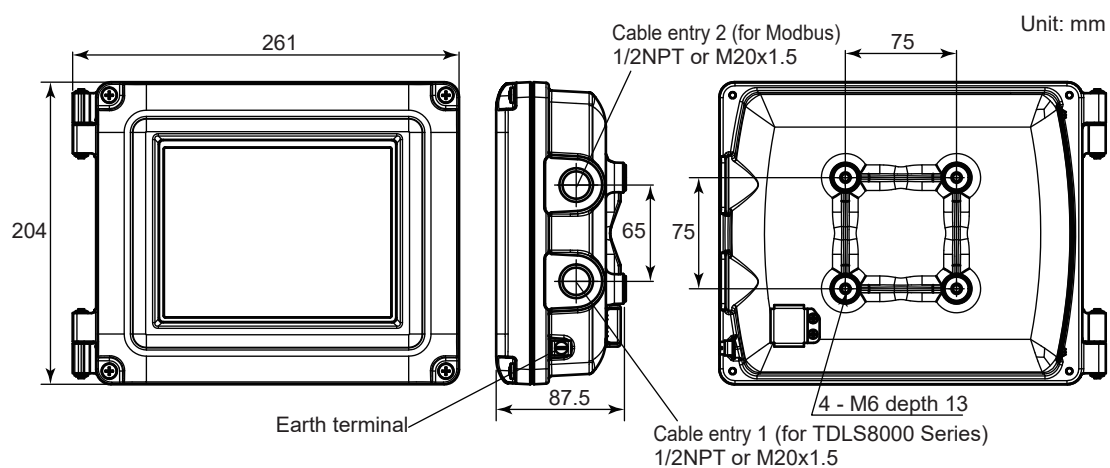


Mounting kit for TDLS8000 series (Option code: /M)

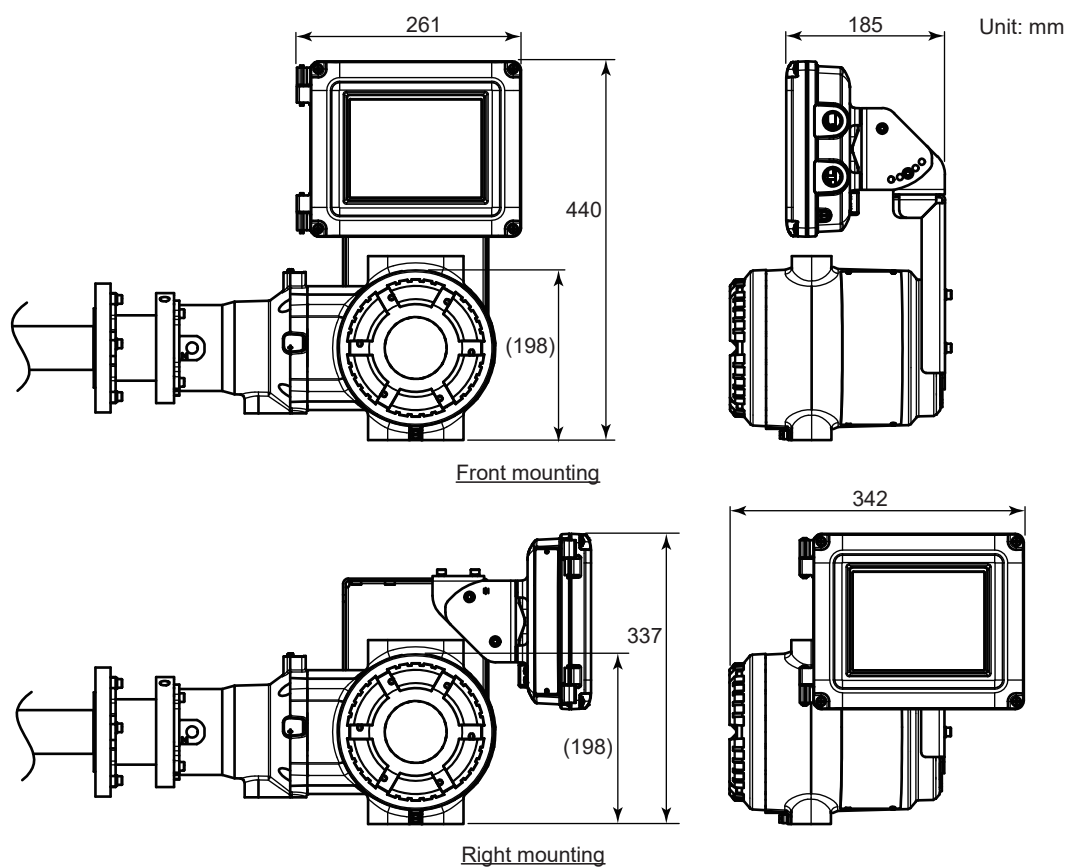

Available for left mounting

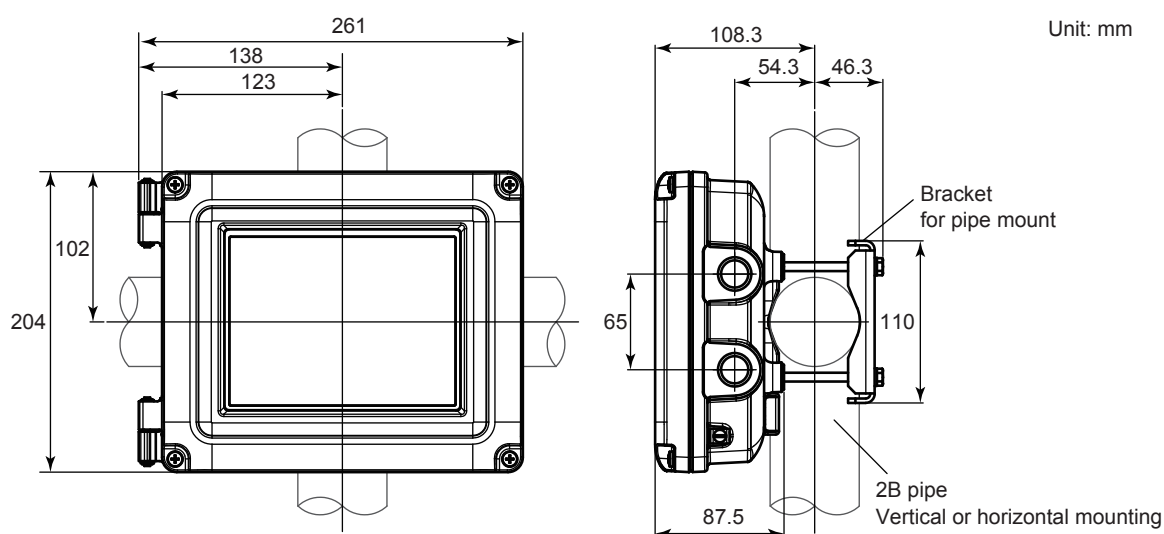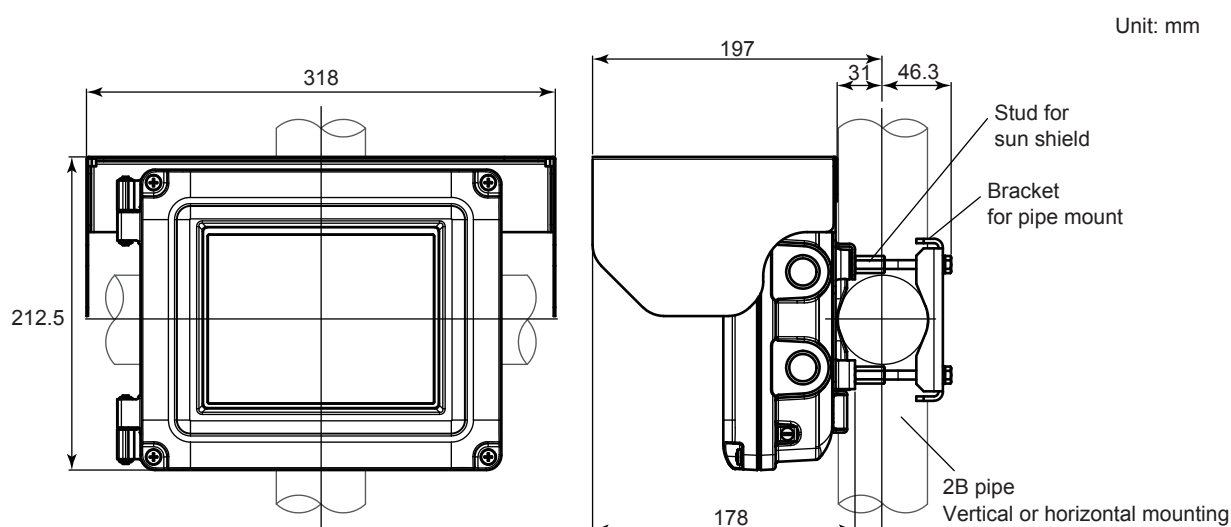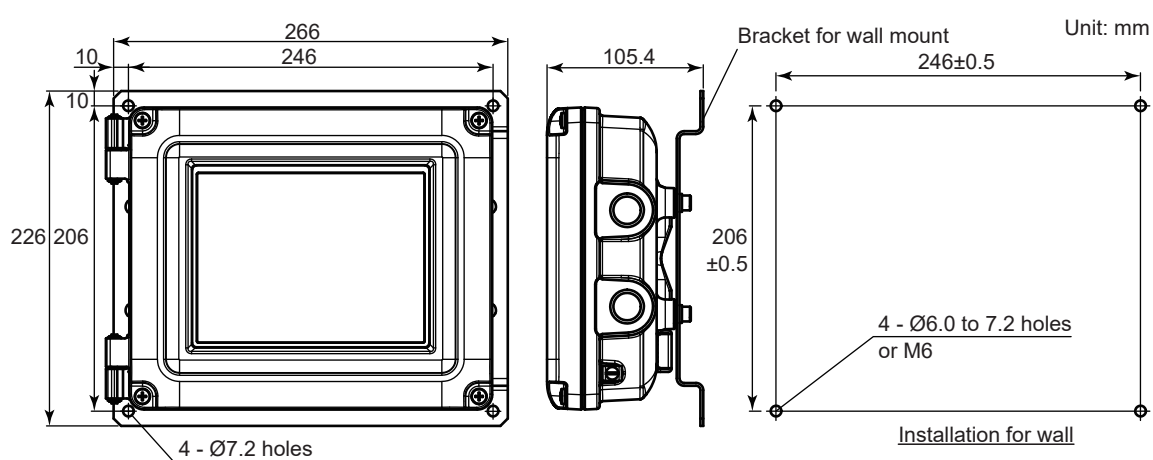Pipe mount (Option code: /P)**Sun Shield (Option code: /S)****Wall mount (Option code: /W)**


*: The wall construction for mounting has to be designed for 4 times the weight of the YH8000.
Bracket for wall mount can be placed in lengthwise

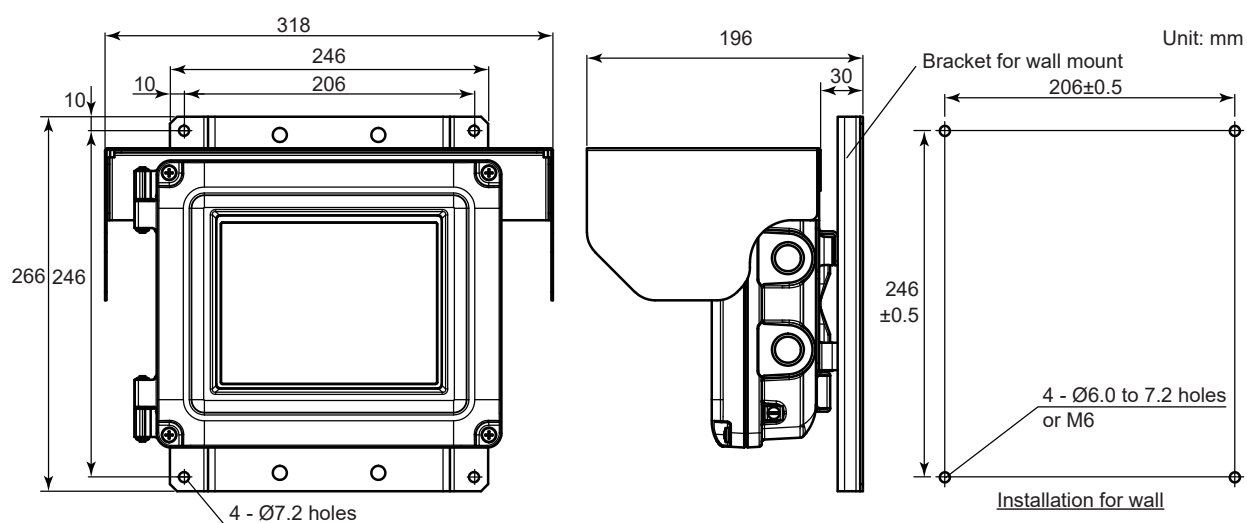Sun Shield (Option code: /S)


When the sun shield is mounted, the bracket for wall have to be placed in widthwise.

■ Calibration Cell

Part number: K9777ZA

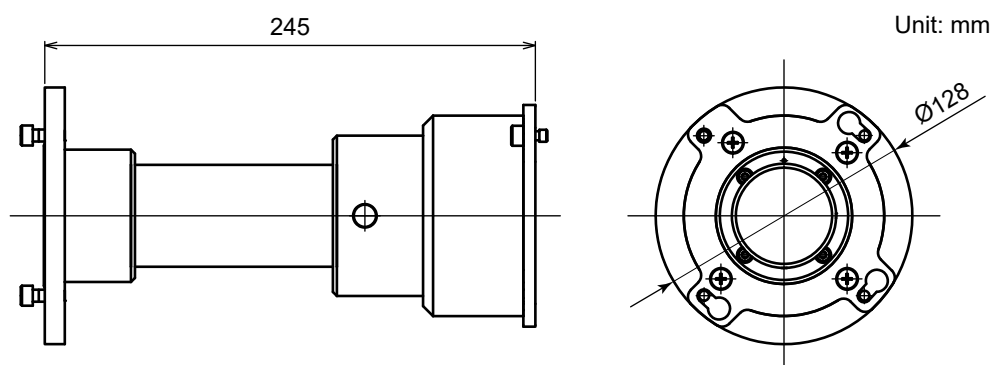


Part number: K9777ZK, K9777ZL

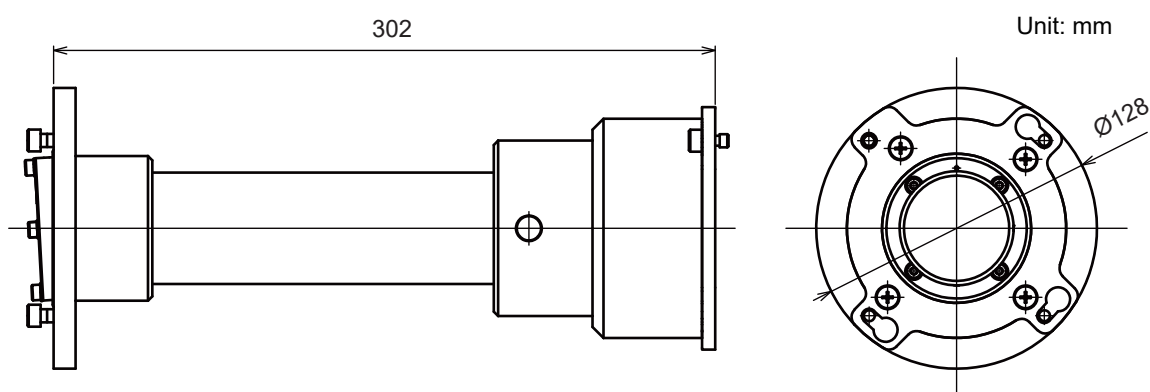


■ WIRING


Wiring the TDLS8100 Probe type Tunable Diode Laser Spectrometer

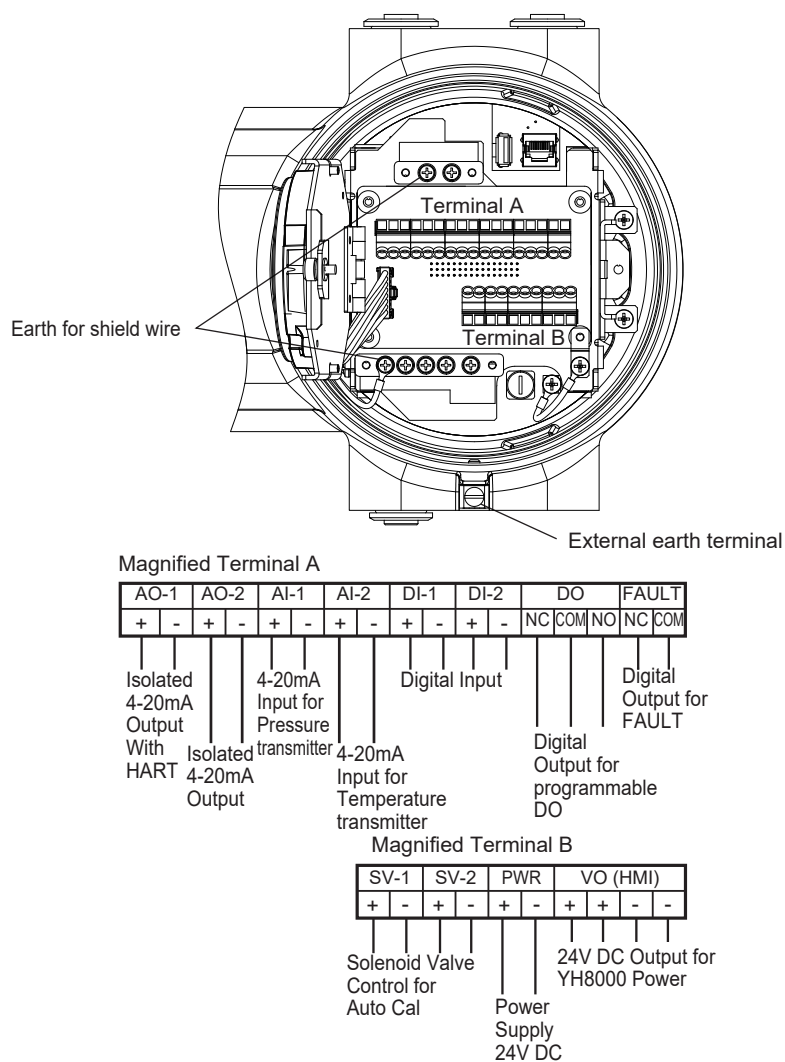

Wiring the YH8000 HMI UNIT

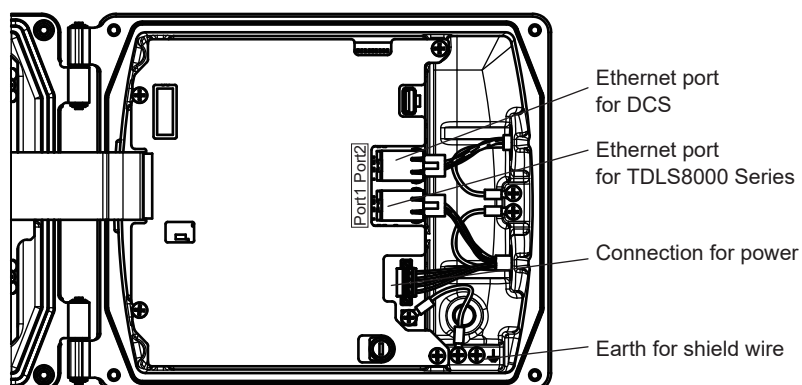


Local HMI configuration

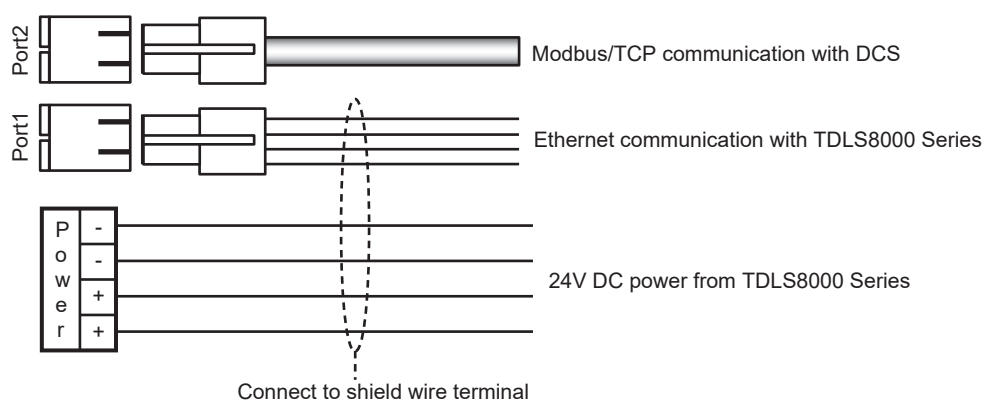

- Connection cable between TDLS8000 Series and YH8000 must be use special cable which can be specified option code "/C."
- Maximum cable length between TDLS8000 Series and YH8000 is 3m.
- Maximum cable length between YH8000 and DCS is 100m.

Remote HMI configuration

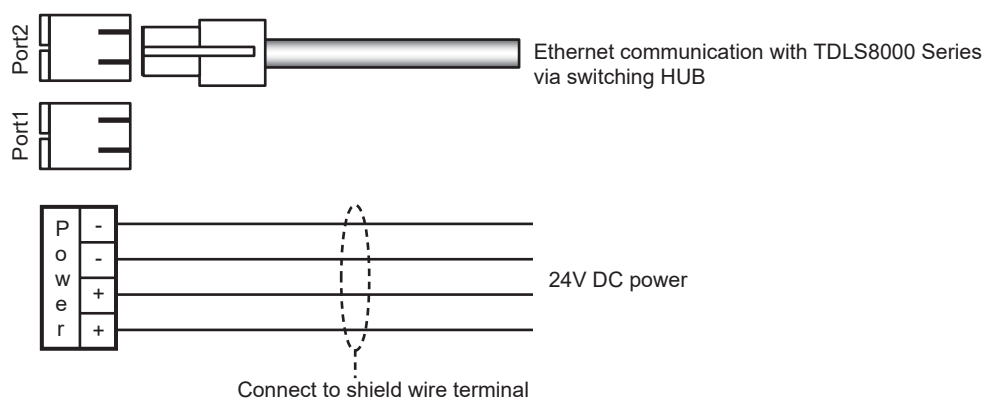

- Maximum cable length between YH8000 and Switching HUB is 100m.