

Instruction Manual

Model FU24
pH/ORP Combination sensor
with pressure compensation



(BG)

Всички улътвания за продукти от серията ATEX Ex се предлагат на английски език. Ако се нуждаете от улътвания за продукти от серията Ex на родния ви език, се свържете с най-близкия офис или представителство на фирма Yokogawa.

(CZ)

Všechny uživatelské příručky pro výrobky, na něž se vztahuje nevýbušné schválení ATEX Ex, jsou dostupné v angličtině. Požadujete-li pokyny týkající se výrobků s nevýbušným schválením ve vašem lokálním jazyku, kontaktujte prosím vaši nejbližší reprezentační kancelář Yokogawa.

(D)

Alle Betriebsanleitungen für ATEX Ex bezogene Produkte stehen in den Sprachen Englisch. Sollten Sie die Betriebs- anleitungen für Ex-Produkte in Ihrer Landessprache benötigen, setzen Sie sich bitte mit Ihrem örtlichen Yokogawa-Vertreter in Verbindung.

(DK)

Alle brugervejledninger for produkter relateret til CE er tilgængelige på engelsk. Skulle De ønske yderligere oplysninger om håndtering af CE produkter på eget sprog, kan De rette henvendelse herom til den nærmeste Yokogawa afdeling eller forhandler.

(EST)

Kõik ATEX Ex toodete kasutamisjuhendid on esitatud inglise keeles. Ex seadmete muuakeelse dokumentatsiooni saamiseks pöörduge lähiima lokagava (Yokogawa) kontori või esindaja poole.

(E)

Todos los manuales de instrucciones para los productos antiexplosivos de ATEX están disponibles en inglés. Si desea solicitar las instrucciones de estos artículos antiexplosivos en su idioma local, deberá ponerse en contacto con la oficina o el representante de Yokogawa más cercano.

(F)

Tous les manuels d'instruction des produits ATEX Ex sont disponibles en langue anglaise. Si vous nécessitez des instructions relatives aux produits Ex dans votre langue, veuillez bien contacter votre représentant Yokogawa le plus proche.

(GB)

All instruction manuals for ATEX Ex related products are available in English. Should you require Ex related instructions in your local language, you are to contact your nearest Yokogawa office or representative.

(GR)

Ολα τα εγχειρίδια λειτουργίας των προϊοντων με ATEX Ex διατίθενται στα Αγγλικά. Σε περιπτώση πων χρειαζεστε οδηγιες σχετικα με Ex στην τοπικη γλωσσα παρακαλομε επικοινωνηστε με το πλησιεστερο γραφειο της Yokogawa η αντιπροσωπο της.

(H)

Az ATEX Ex műszerek gépkönyveit angol nyelven adjuk ki. Amennyiben helyi nyelven kérík az Ex eszközök leírásait, kérjük keressék fel a legközelebbi Yokogawa irodát, vagy képviseletet.

(I)

Tutti i manuali operativi di prodotti ATEX contrassegnati con Ex sono disponibili in inglese. Se si desidera ricevere i manuali operativi di prodotti Ex in lingua locale, mettersi in contatto con l'ufficio Yokogawa più vicino o con un rappresentante.

(LV)

Visas ATEX Ex kategorijas izstrādājumu Lietoðanas instrukcijas tiek piegādātas angīu valodās. Ja vçlaties saðemt Ex ierïeu dokumentāciju citā valodā, Jums ir jåsazinâs ar firmas Yokogawa (Yokogawa) tuvâko ofisu vai pârstâvi.

(LT)

Visos gaminiø ATEX Ex kategorijos Eksplotavimo instrukcijos teikiami anglø kalbomis. Norëdami gauti priestaisø Ex dokumentacijà kitomis kalbomis susisiekite su artimiausiu bendrovës Yokogawa biuru arba atstovu.

(M)

Il-manwali kollha ta' l-istruzzjonijiet ghal prodotti marbuta ma' ATEX Ex huma disponibbli bl-Ingliz. Jekk tkun tehtieß struzzjonijiet marbuta ma' Ex fil-lingwa lokali tiegħek, għandek tikkuntattja lill-eqreb rappreżentan jew uffiċċju ta' Yokogawa.

(NL)

Alle handleidingen voor producten die te maken hebben met ATEX explosiebeveiliging (Ex) zijn verkrijgbaar in het Engels. Neem, indien u aanwijzingen op het gebied van explosiebeveiliging nodig hebt in uw eigen taal, contact op met de dichtstbijzijnde vestiging van Yokogawa of met een vertegenwoordiger.

(P)

Todos os manuals de instruções referentes aos produtos Ex da ATEX estão disponíveis em Inglês. Se necessitar de instruções na sua língua relacionadas com produtos Ex, deverá entrar em contacto com a delegação mais próxima ou com um representante da Yokogawa.

(PL)

Wszystkie instrukcje obsługi dla urządzeń w wykonaniu przeciwwybuchowym Ex, zgodnych z wymaganiami ATEX, dostępne są w języku angielskim. Jeżeli wymagana jest instrukcja obsługi w Państwa lokalnym języku, prosimy o kontakt z najbliższym biurem Yokogawy.

(RO)

Toate manualele de instructiuni pentru produsele ATEX Ex sunt in limba engleza. In cazul in care doriti instructiunile in limba locala, trebuie sa contactati cel mai apropiat birou sau reprezentant Yokogawa.

(S)

Alla instruktionsböcker för ATEX Ex (explosionssäkra) produkter är tillgängliga på engelska. Om Ni behöver instruktioner för dessa explosionssäkra produkter på annat språk, skall Ni kontakta närmaste Yokogawa kontor eller representant.

(SF)

Kaikkien ATEX Ex-tyypistien tuotteiden käyttöohjeet ovat saatavilla englannin-. Mikäli tarvitsette Ex-tyypistien tuotteiden ohjeita omalla paikallisella kielellännne, ottakaa yhteyttä lähimpään Yokogawa-toimistoon tai -edustajaan.

(SK)

Všetky návody na obsluhu pre prístroje s ATEX Ex sú k dispozícii v jazyku anglickom. V prípade potreby návodu pre Ex-prístroje vo Vašom národnom jazyku, skontaktujte prosím miestnu kanceláriu firmy Yokogawa.

(SLO)

Vsi predpisi in navodila za AEX Ex sorodni pridelki so pri roki v angleščini. Če so Ex sorodna navodila potrebna v vašem tukejnjem jeziku, kontaktirajte vaš najbližji Yokogawa office ili predstanika.

CONTENTS

1. PREFACE	6
1.1 Introduction	6
1.2 Unpacking and Checking	6
1.3 Warranty and Service	7
1.4 Serial number	7
2. GENERAL SPECIFICATIONS	8
2.1 Measuring elements	8
2.2 Wetted parts	8
2.3 Functional specifications (at 25°C)	8
2.4 Dynamic specifications	8
2.5 Operating range	8
2.6 Regulatory standards	9
2.7 Shipping details	9
2.8 Environmental conditions	9
2.9 Mechanical specifications	9
3. INSTALLATION OF FU24	10
3.1 Typical installation	10
3.2 Preparing the sensor for use	10
3.3 Mounting the sensor	10
4. DIMENSIONS	12
5. WIRING	13
5.1 Connections	13
5.2 Definition EXA/FLXA terminal numbers to FU24 sensor	13
5.3 Settings for PH402G and PH202G(S)	14
5.4 Settings for PH150, PH450G and FLXA	14
6. GENERAL CALIBRATION & MAINTENANCE PROCEDURE	14
6.1 Calibration for pH measurement	14
6.2 Calibration for ORP and rH measurement	15
6.3 Maintenance of the FU24 sensor	15
7. MODEL CODES	16
8. SPARE PARTS	16
9. CHEMICAL COMPATIBILITY CHART	17

1. PREFACE

1.1 Introduction

This instruction manual provides information for the installation and use of the FU24 four-in-one wide body pH sensor, which is especially designed for harsh process applications.

The Model FU24 offers a simple and cost effective solution for process applications with fluctuating pressure and/or temperature which normally limit the lifetime of a sensor.

By using the patented Bellow system a strong pressure compensation mechanism is created. This ensures immediate interior pressure equalization to the outside process pressure, making the sensor virtually insensitive to process pressure variations.

A slight overpressure caused by the bellow tension prevents process fluid ingress and maintains a positive ion flow out of the sensor. This feature is of particular interest in pure water applications.

This all-in-one sensor provides simultaneous measurement of pH, redox (ORP) and temperature if desired. The rugged PPS 40GF (Ryton™) body is designed for easy installation via the 1" NPT threaded connections provided on both ends of the sensor.

The FU24 comes with an integral cable of optional lengths designed to minimize the adverse affects noise can have on the measurement. This cable is pre-finished to make connection to any industrial pH instrument as simple as possible. The FU24 can also include a multipole VP connector and then requires separate cable type WU10-V-S that is available in 5 fixed lengths.

1.2 Unpacking and Checking

Upon delivery, unpack the sensor carefully and inspect it to ensure it was not damaged during shipment. If damage is found, retain the original packing materials and then immediately notify the carrier and the relevant Yokogawa sales office. Make sure the Model Code and Serial Number on the sensor are the same as on the packing list. Also, check any option(s) that were ordered are included and correct.

1.3 Warranty and Service

Yokogawa products and parts are guaranteed free from defects in workmanship and material under normal use and service for a period of (typically) 12 months from the date of shipment from the manufacturer. Individual sales organizations can deviate from the typical warranty period, and the conditions of sale relating to the original purchase order should be consulted. Damage caused by wear and tear, inadequate maintenance, corrosion, or by the effects of chemical processes are excluded from this warranty coverage. In the event of warranty claim, the defective goods should be sent (freight paid) to the Service Department of the relevant sales Organization for repair or replacement (at Yokogawa's discretion).

The following information must be included in the letter accompanying the returned goods:

- Model Code and Serial Number.
- Original Purchase Order and Date.
- Length of time in service and description of the process.
- Description of the fault and circumstances of the failure.
- Process/environmental conditions that may be related to the failure of the sensor
- Statement as to whether warranty or non-warranty service is requested.
- Complete shipping and billing instructions for return of material, plus the name and phone number of a contact person that can be reached for further information.
- Clean Statement
Returned goods that have been in contact with process fluids must be decontaminated and disinfected prior to shipment. Goods should carry a certificate to this effect, for the health and safety of our employees. Material Safety Data sheets must be included for all components of the process to which the sensor(options) have been exposed.

1.4 Serial number

The Serial number is defined by nine (9) alphanumeric characters:

X ₁ X ₂	Production location
X ₃ X ₄	Year/Month code
X ₅ X ₆ X ₇ X ₈ X ₉	Tracking number

Example: N3P600028

Table 1:

Year	Yearcode	Year	Yearcode
2014	P	2026	3
2015	R	2027	4
2016	S	2028	5
2017	T	2029	6
2018	U	2030	7
2019	V	2031	8
2020	W	2032	9
2021	X	2033	A
2022	Y	2034	B
2023	Z	2035	C
2024	1	2036	D
2025	2	2037	E

Table 2:

Month	Monthcode
January	1
February	2
March	3
April	4
May	5
June	6
July	7
August	8
September	9
October	A
November	B
December	C

2. GENERAL SPECIFICATIONS

2.1 Measuring elements

- : pH glass electrode
- : Silver chloride reference
- : Solid platinum electrode
- : Pt1000 temperature sensor.

2.2 Wetted parts

Sensor body	: PPS 40GF (Ryton™ with glass filling)
Earthing pin	: Solid Platinum
Measuring sensor	: G-glass
LE glass tube	: AR-glass
O-ring	: Viton
Reference junction	: Porous PTFE
Bellow system	: Viton

2.3 Functional specifications (at 25°C)

Isothermal point	: pH 7
Reference system	: Ag/AgCl with saturated KCl
Glass impedance	
- Dome shape	: 100 MΩ nominal
- Flat Surface	: 500 MΩ nominal
Junction resistance	: 1.0 to 15 kΩ
Liquid outlet	: non-flow double junction
Temperature element	: Pt1000 to IEC 751
Asymmetry potential	: 8 ± 15 mV
Slope	: > 96 % (of theoretical value)


Note: The temperature sensor included in the FU24 is designed for cell compensation and for indication. It is **NOT** designed for process temperature control.

2.4 Dynamic specifications

Response time pH	: $t_{90} < 15$ sec. (for 7 to 4 pH step)
Response time temperature	
- Dome shape	: $t_{90} < 1$ min. (for 10 °C step)
- Flat surface	: $t_{90} < 4$ min. (for 10 °C step)
Stabilization time pH	: < 2 min. (for 0.02 pH unit during 10 sec.)

2.5 Operating range

pH	: 0 to 14
ORP	: -1500 to 1500 mV
rH	: 0 to 100
Temperature	
- Dome shape	: -10 to 105 °C (14 to 221 °F)
- Flat Surface	: +15 to 105 °C (59 to 221 °F)
Pressure	: p(bar)

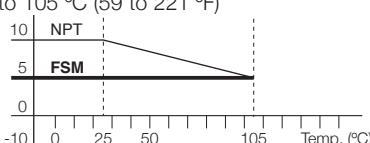

Conductivity : > 10 µS/cm

Note: The pH operating range at room temperature is 0-14 pH, but at high temperatures or range outside 2-12 pH the lifetime will be seriously shortened.

Note: Sensor is suitable for pure water applications

2.6 Regulatory standards

CE	: Decision 768/2008/EC 
- ATEX	: Directive 2014/34/EU, as amended by Regulation (EC) no. 1882/2003
Certificate no.	: DEKRA 11ATEX0014 X  II 1 G Ex ia IIC T3...T6 Ga
Electrical data	: For sensor input circuit connected to a certified intrinsically safe circuit with the following maximum values: Ui = 18 V; Ii = 170 mA; Pi = 0.4 W; Li = 0 mH; Ci = 0 nF (VP type) or 3.6 nF (permanently connected cable) or Certified intrinsically safe Yokogawa pH/ORP transmitter Model FLXA21 series or Model PH202S series.
Special conditions (X)	: T6 for Tamb. -40 °C to +40 °C T4 and T5 for Tamb. -40 °C to +55 °C T3 for Tam. -40 °C to +105 °C
 WARNING	: Electrostatic charges on the sensor enclosure shall be avoided.
- Pressure	: Directive 2014/68/EU, as amended by Regulation (EC) no. 1882/2003
Applying article	: 4.3 (Sound Engineering Practice) : Damaging the screw thread of the sensor might influence the maximum process pressure. : Sensor contains glass parts which if broken can cause cutting injuries.
 WARNING	
IECEx	
Applying standards	: IEC 60079-0: 2007 IEC 60079-11: 2006 IEC 60079-26: 2006
Certificate no.	: IECEx DEK 11.0064X Ex ia IIC T3...T6 Ga

Note: When the sensor has been connected to none intrinsically safe equipment which exceeds the restrictions regarding the sensor input circuit (see electrical data), the sensor is not suitable anymore for intrinsically safe use.

2.7 Shipping details

Package size (LxWxH)	FU24-05/10	FU24-VP
	410x130x75 16.1x5.1x3.0	300x100x75 mm 11.8x3.9x3.0 inch
Package weight (max.)	0.92 kg (2.02 lbs)	0.33 kg (0.73 lbs)

2.8 Environmental conditions

Storage temperature	: -10 to 50 °C (14 to 122 °F)
Water proof	: IP67 (conform IEC 60529)

2.9 Mechanical specifications

Max. torque on sensor body: 7,5 Nm

3. INSTALLATION OF FU24

For optimum measurement results, the FU24 should be installed in a location that offers an acceptable representation of the process composition and **DOES NOT** exceed the specifications of the sensor. The FU24 is designed with 1" NPT threaded connections on both ends of the sensor to allow installation in a wide variety of applications.

3.1 Typical installation

The FU24 sensor is designed for versatile in-line, immersion or bypass loop installation. For best results the FU24 should be mounted with the process flow coming towards the sensor. The sensor can be mounted in all angles with respect to the horizontal plane.

3.2 Preparing the sensor for use

Remove the sensor from its shipping box and slide off the so-called 'wet pocket', the tube filled with solution to prevent drying out of the measuring elements during shipment or storage. It is recommended to calibrate the sensor before first use.

A general calibration procedure is described in Section 6 of this Instruction Manual.

3.3 Mounting the sensor

The simplest mounting is to use one of the 1" NPT threaded connection of the sensor. Apply Teflon tape to the appropriate threaded end, then install the sensor in the process. Tighten the sensor using a wrench on the sensor flats.

The FU24 can also be mounted in a FF20-*22 and FF20-*33 flow fitting or put in the process by making use of the FS20-*22 and FS20-*32 subassembly. In both cases this can be realized by using one of the spare part adapters (see Section 8 for ordering information).

- 1 Apply Teflon tape to the threaded end of the sensor;
- 2 Install the sensor in the adapter. Tighten the sensor using a wrench on the sensor flats (see Figure 1 and 2).

Note: **DO NOT** over tighten the sensor to prevent damage. The maximum applicable torque is 7,5 Nm.

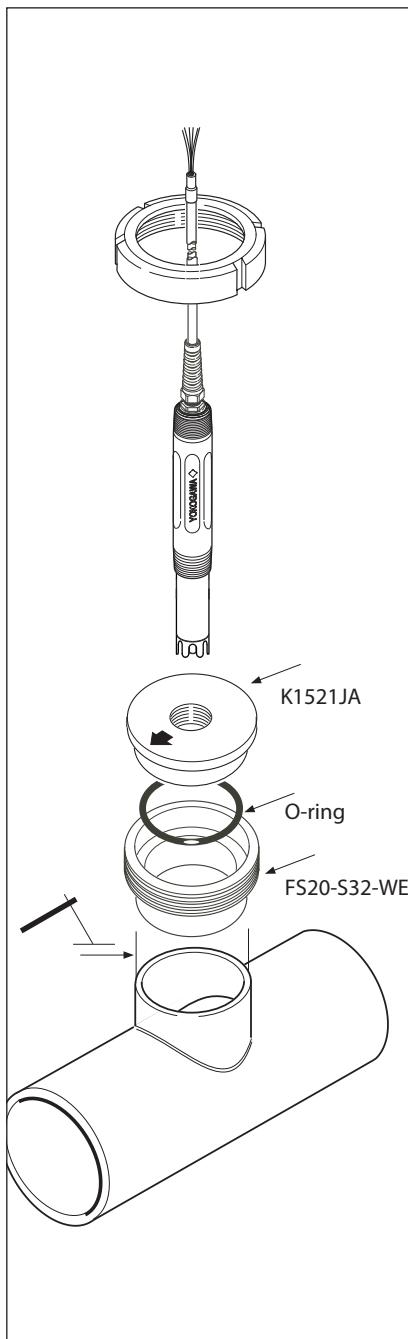


Figure 1. FS20 installation example FU24

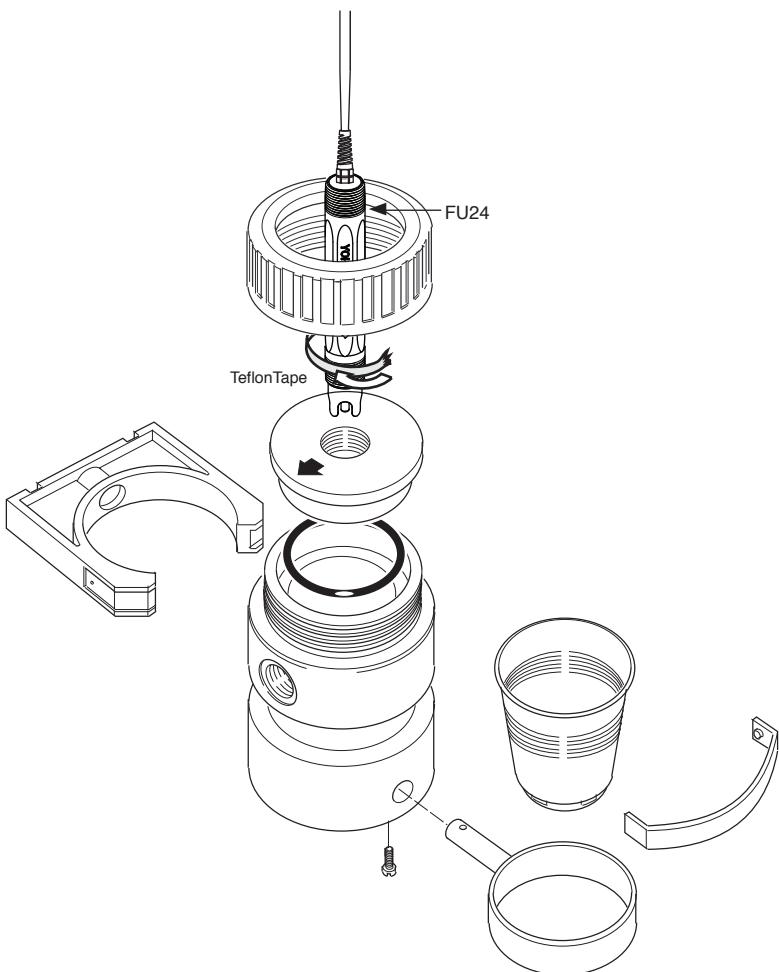


Figure 2. FF20-33 installation example FU24

4. DIMENSIONS

Dimensions in mm (inches)

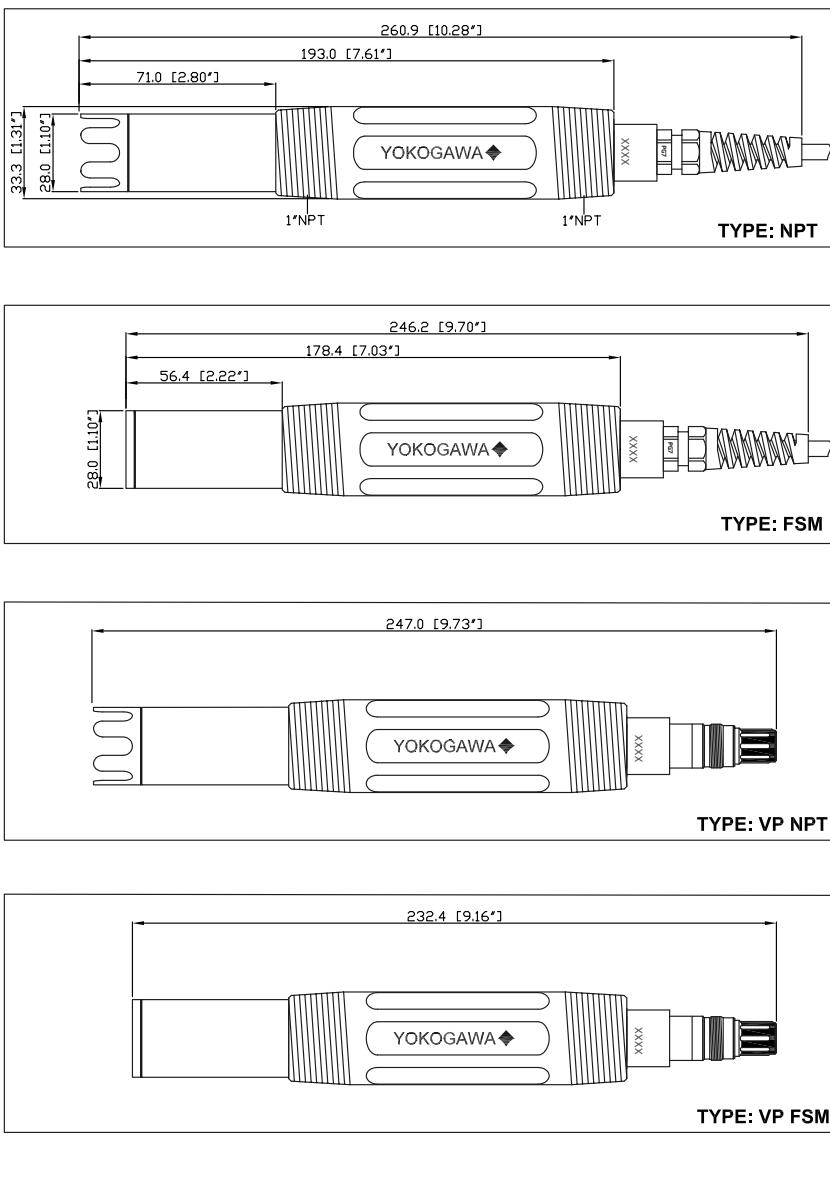


Figure 3. Dimensions FU24

5. WIRING

5.1 Connections

The FU24 sensor is provided with a fixed cable or Variopin (VP) connector. The connections of both the wire as the VP connector are given in Figure 4.

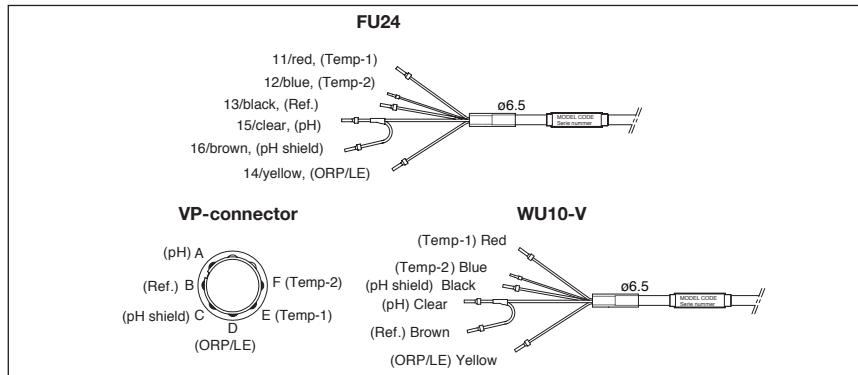


Figure 4. Cable marking and pin locations

5.2 Definition EXA/FLXA terminal numbers to FU24 sensor

FU24-05/10 wire #			
EXA/FLXA terminal #	pH pH+ORP pH+rH	ORP	ORP pH compensated
11	11	11	11
12	12	12	12
13	13	13	15
14	14		
15	15	14	14
16	16		
17			16

FU24-VP with WU10-V wire color			
EXA/FLXA terminal #	pH pH+ORP pH+rH	ORP	ORP pH compensated
11	Red	Red	Red
12	Blue	Blue	Blue
13	Brown	Brown	Clear
14	Yellow		
15	Clear	Yellow	Yellow
16	Black		
17			Black

Note: For ORP measurement the EXA/FLXA terminals 13 and 14 should be interconnected.
For ORP pH compensated measurement the EXA/FLXA terminals 14 and 15 should be interconnected.

5.3 Settings for PH402G and PH202G(S)

Function Setting	pH (default)	pH&ORP	pH&rH	ORP	pH compensated ORP
code 01	0(pH)	0(pH)	0(pH)	1(ORP)	1(ORP)
code 02	0(off)	1(ORP)	2(rH)	0(off)	0(off)
code 03	1.1.1	1.1.1	1.1.1	0.0.1	0.0.1
code 04	0.0.1	0.0.1	0.0.1	0.0.1	1.1.1
code 31	0	2	2		
jumper input 1	no	no	no	yes	yes
jumper input 2	yes	yes	yes	yes	no

5.4 Settings for PH150, PH450G and FLXA

Function Setting	pH (default)	pH&ORP	pH&rH	ORP	pH compensated ORP
sensor setup	pH	pH+ORP	pH+ORP	ORP	ORP
measurement setup		pH+ORP	pH+rH		
Impedance setting					
input1	High	High	High	Low	Low
input 2	Low	Low	Low	Low	High
jumper input 1	no	no	no	yes	yes
jumper input 2	yes	yes	yes	yes	no

6. GENERAL CALIBRATION & MAINTENANCE PROCEDURE

6.1 Calibration for pH measurement

To calibrate the FU24 pH/ORP sensor, two buffer solutions with known pH values are required. It is recommended that one buffer solution has a value near to pH 7.00. Depending on the process value to be measured, the second buffer solution should be either acidic (below pH 7.00) or alkaline (above pH 7.00). Normally the IEC buffers (pH 4.01, 6.87 and 9.18) are used.

The following is a very general 2-point calibration procedure:

1. Clean the sensor using a 5% solution of HCl;
2. Rinse sensor thoroughly with demineralized water;
3. Immerse the sensor in the first buffer (pH 6.87 is recommended) and execute calibration as described in the Instruction Manual of the analyzer.
4. Rinse sensor thoroughly with demineralized water;
5. Immerse the sensor in the second buffer (pH 4.01 or 9.18 is recommended) and execute calibration as described in the Instruction Manual of the analyzer.
6. Rinse sensor thoroughly with demineralized water.

During calibration, the temperature compensation should be active.

The EXA/FLXA analyzer automatically compensates for the sensitivity change of the pH sensor at different temperatures.

After calibration, replace or re-install the sensor into the process.

6.2 Calibration for ORP and rH measurement

For calibration of ORP and rH, the procedure for MANUAL CALIBRATION can be used as described in the Instruction Manual of the analyzer.

The rH value is a function of the reference system and the pH value of the buffer solution. The FU24 sensor has a reference system of saturated Silver/Silver Chloride (Ag/AgCl). The commonly used standards for ORP and rH calibration are made from Chinhydron (Quinhydrone) powder dissolved in pH buffer solutions (1 g / 200 ml). In Table 3 the measurement values are given as function of the used pH buffer solution with Chinhydron powder. The accuracy of the standards is approximately ± 10 mV.

Table 3: ORP, pH compensated ORP and rH as function of pH buffer solution with Chinhydron powder.

pH buffer	ORP (mV) ORP (mV)	pH compensated	rH
1.68	403	88	23.6
4.01	265	88	23.6
6.87	96	88	23.6
7.00	88	88	23.6

6.3 Maintenance of the FU24 sensor

A pH sensor requires routine maintenance to keep the measuring elements clean and functioning. Depending on the process, different cleaning solutions may be required.



Avoid cleaning the complete sensor with solution. Some cleaning solutions will damage the modelcode sticker and connector which are placed on top of the sensor. Only clean the measuring elements at the bottom side of the sensor.

In most cases cleaning with water, iso-propanol or methanol is sufficient. In other cases the measuring elements of the sensor have to be cleaned with specific solutions.

Examples:

1. Deposits of limes, hydroxides or carbonates can be removed by immersing the bottom part of the sensor in a solution containing dilute hydrochloric acid (5% is recommended). Afterwards rinse the sensor with water.
2. Deposits of oil and fat can be removed with hot water with a detergent. When the results are unsatisfactory, a mild (carbonate based) abrasive can be used.
3. Protein deposits should be removed with a protein enzymatic solution, for instance a solution containing 8.5 mL concentrated hydrochloric acid and 10 grams of pepsin in 1 liter of water.

Note: Avoid cleaning with non-polar solvent like tri-chloro ethylene, toluene or hexane. The non-polar solvents will break up the gel-layer on the pH glass bulb and requires that the sensor has to be soaked in water for at least 12 hours before it will function again.

The Teflon diaphragm of the sensor can be regenerated by putting it in hot ($\pm 70^\circ\text{C}$, 158°F) 3 molar Potassium Chlorine (KCl) solution and letting it cool down to room temperature. This procedure clears the diaphragm and will soak the diaphragm with conductive KCl again.

7. MODEL CODES

Model Code	Suffix Code	Option	Description
FU24			Wide body sensor
Type	- VP - 05 - 10		Variopin connector Fixed cable, 5 meter Fixed cable, 10 meter
Temp. element	- T1		Pt1000
Model	- NPT - FSM		Dome shape model Flat surface model

8. SPARE PARTS

Spare part	Description
FU24	
K1521JA	SS holder 1" NPT
K1521JB	PVDF holder 1" NPT
Buffer solutions	
K1520BA	Starters Kit: (3x 500 ml) Solution pH 4.01, pH 6.87, pH 9.18
K1520BB	Buffer Solution (500 ml) pH 1.68
K1520BC	Buffer Solution (500 ml) pH 4.01
K1520BD	Buffer Solution (500 ml) pH 6.87
K1520BE	Buffer Solution (500 ml) pH 9.18
Connection equipment	
BA10	Junction box for pH extension cables
WF10-XXX-F	pH signal cable with terminated ends.
	Available lengths (XXX = 005, 010, 025 & 050 m)
WU10-V-S-XX	Variopin cable (XX = 02, 05, 10, 15 and 20m)

9. CHEMICAL COMPATIBILITY CHART

		Material									
		Viton		PTFE (teflon)		PPS (Ryton)	Glass				
		Conc.%	Temp. °C	20	60	100	20	60	100	20	60
Inorganic acid	Sulfuric acid	10		O	O	O	O	O	O	O	O
		50		O	O	O	O	O	X	X	O
		95		O	O	O	O	O	X	X	-
		fuming		O	O	O	O	O			O
	Hydrochloric acid	10		O	O	O	O	O	O	O	O
		sat.		O	O	O	O	O	O	O	O
	Nitric acid	25		O	O	X	O	O	O	O	O
		50		-	-	-	O	O	X	X	O
		95		-	-	-	O	O	-	-	O
		fuming		-	-	-	O	O	O		O
Organic acid	Phosphoric acid	25		O	O	O	O	O	O	O	O
		50		O	O	O	O	O	O	O	O
		95		X	X	-	O	O	O	O	O
	Hydrofluoric acid	40		O	O	O	O	O	X	X	X
		75		O	O	X	O	O	-	-	-
	Acetic acid	10		-	-	-	O	O	O	O	O
		glacial		-	-	-	O	O	O	O	O
		Formic acid		80	-	-	O	O	O	O	O
Alkali	Citric acid	50		O	O	O	O	O	O	O	O
		Calcium hydroxide		sat.	O	O	O	O	O	O	O
	Potassium hydroxide	50		O	O	O	O	O	O	O	X
	Sodium hydroxide	40		X	X	X	O	O	O	O	X
	Ammonia in water	30		X	X	X	O	O	O	O	X
Acid salt	Ammonium chloride	sat.		O	O	O	O	O	O	O	O
	Zinc chloride	50		O	O	O	O	O	O	O	O
	Iron(III) chloride	50		O	O	O	O	O	O	O	O
	Sodium sulfite	sat.		-	-	-	O	O	O	O	O
Basic salt	Sodium carbonate	sat.		O	O	O	O	O	O	O	O
	Potassium chloride	sat.		O	O	O	O	O	O	O	O
	Sodium sulfate	sat.		O	O	O	O	O	O	O	O
	Calcium chloride	sat.		O	O	O	O	O	O	O	O
	Sodium chloride	sat.		O	O	O	O	O	O	O	O
Neutral salt	Sodium nitrate	50		O	O	O	O	O	O	O	O
	Aluminium chloride	sat.		O	O	O	O	O	O	O	O
	Hydrogen peroxide	30		O	O	O	O	O	X	-	O
	Sodium Hypochlorite	50		O	O	X	O	O	O	O	O
Oxidizing agent	Potassium dichromate	sat.		O	O	O	O	O	X	O	O
	Chlorinated lime						O	O	O	O	O
	Ethanol	80		X	-	-	O	O	O	O	O
	Cyclohexane			O	O	O	O	O	O	O	O
Organic solvent	Toluene			-	-	-	O	O	O	O	O
	Trichloroethane			X	X	X	O	O	O	O	O
	Water			O	O	O	O	X	O	O	O

O = can be used; X = shortens useful life; - = cannot be used; Blank = no data available

Note: Information in this list is based on our general experience and literature data and given in good faith. However Yokogawa is unable to accept responsibility for claims related to this information.

YOKOGAWA ELECTRIC CORPORATION
World Headquarters
9-32, Nakacho 2-chome, Musashino-shi
Tokyo 180-8750
Japan
www.yokogawa.com

YOKOGAWA CORPORATION OF AMERICA
2 Dart Road
Norcross GA 30265
USA
www.yokogawa.com/us

YOKOGAWA EUROPE BV
Europe 2
3025 HD AMERSFOORT
The Netherlands
www.yokogawa.com/eu

YOKOGAWA ELECTRIC ASIA Pte. LTD.
5 Bedok South Road
Singapore 469270
Singapore
www.yokogawa.com/sg

YOKOGAWA CHINA CO. LTD.
37 Tianshan D Cantele Crocodile Building
No.569 Wenzhou Tianshan Road Changning District
Shanghai, China
www.yokogawa.com/cn

YOKOGAWA MIDDLE EAST B.S.C.(c)
P.O. Box 10070, Manama
Building 57, Road 2516, Busaiteen 225
Muharraq, Bahrain
www.yokogawa.com/bh

Yokogawa has an extensive sales and distribution network.
Please refer to the European website (www.yokogawa.com/eu) to contact your nearest representative.



YOKOGAWA ♦