
Drawings

GD80
Gas Density Meter Detector

☐ /PI **Horizontal Mounting with Pipe Mounting Hardware**
Installation is possible in either direction.

Unit：mm

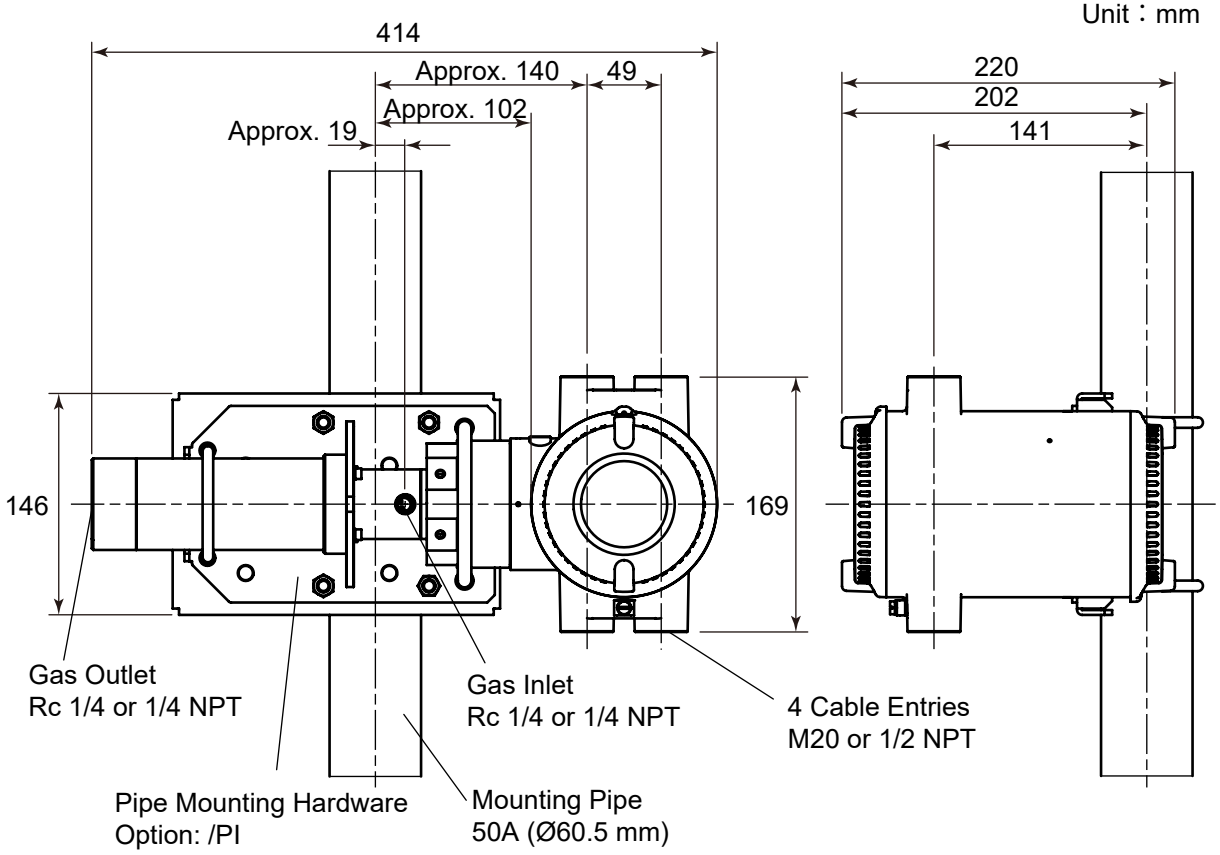


Weight: Approx. 8.5 kg (Detector only)

Unless otherwise specified, differences in the dimensions are specified as: General tolerance = ±(Criteria of tolerance class IT18 in JIS B0401-1998)/2.

All Rights Reserved, Copyright © 2026, Yokogawa Electric Corporation.
Subject to change without notice.

☐ /PI **Vertical Mounting with Pipe Mounting Hardware**

Unit：mm

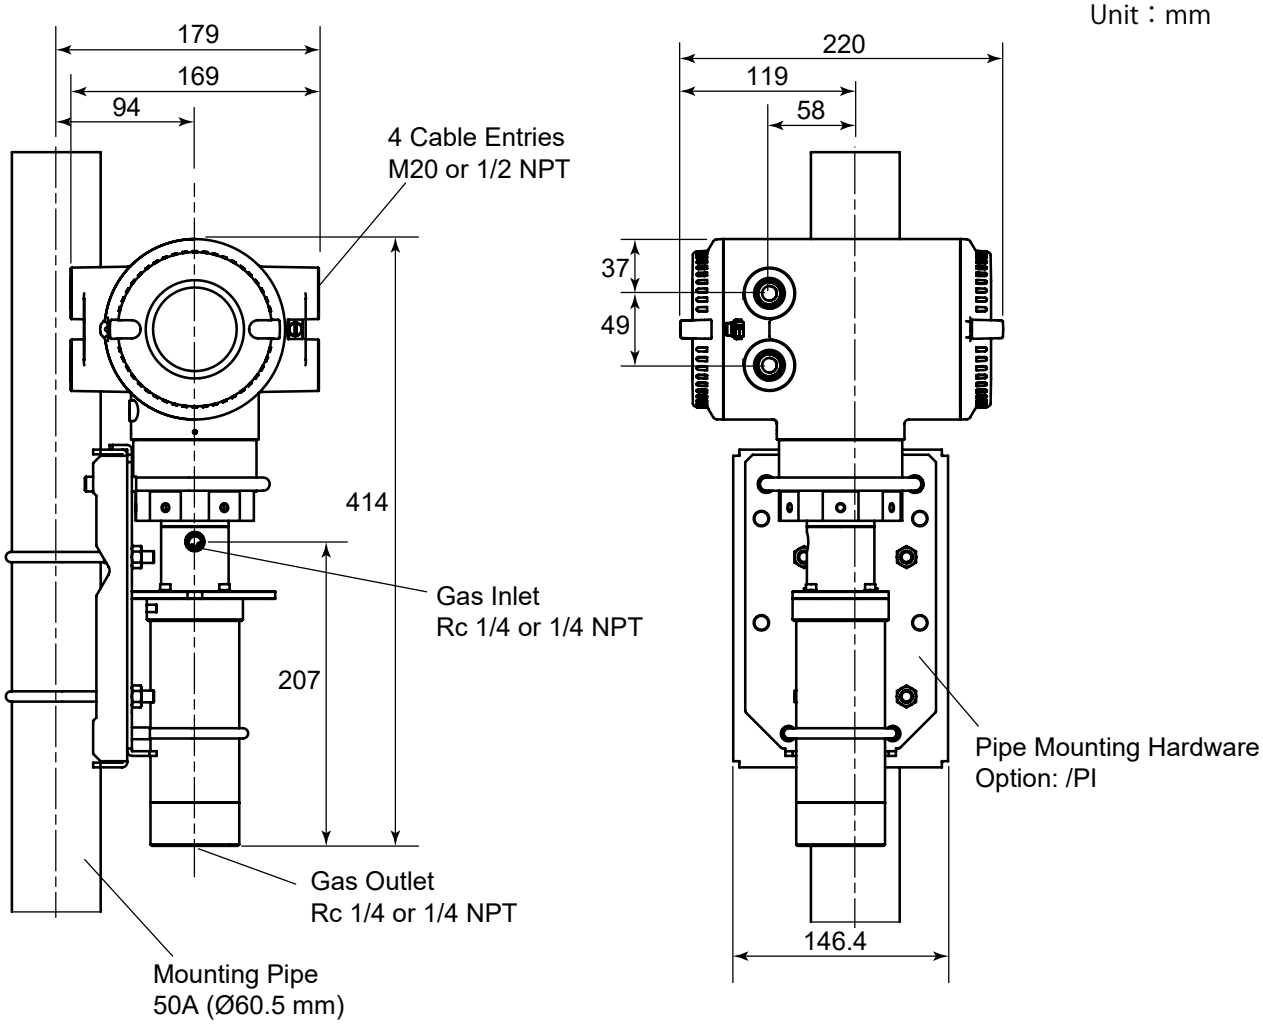


Weight: Approx. 8.5 kg (Detector only)

Unless otherwise specified, differences in the dimensions are specified as: General tolerance = ±(Criteria of tolerance class IT18 in JIS B0401-1998)/2.

☐ /DUH ☐ /DUHT ☐ /DHM* **Detector on Mounting Plate, Horizontal Mounting**

*: For /DHM, only the detector is mounted on the mounting plate. The pressure transmitter must be ordered separately.

Unit：mm

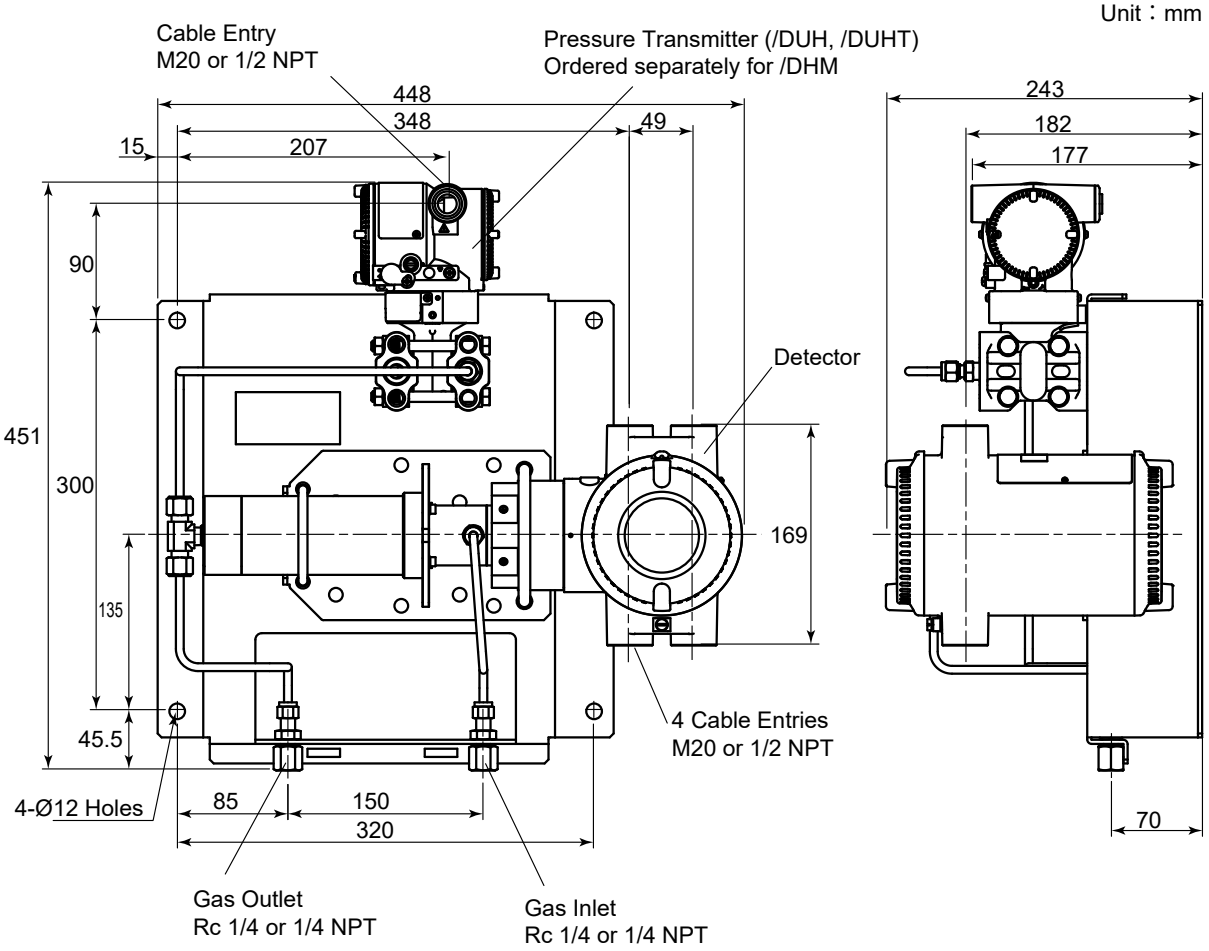

Note: Install the detector at a location capable of supporting the total weight of the detector mounted on the mounting plate (approx. 15.6 kg), cable glands, cables, and other associated components.


Weight: Approx. 15.6 kg (with mounting plate and EJX310A)

Unless otherwise specified, differences in the dimensions are specified as: General tolerance = ±(Criteria of tolerance class IT18 in JIS B0401-1998)/2.

☐ /DUV ☐ /DUVT ☐ /DVM* **Detector on Mounting Plate, Vertical Mounting**

*: For /DVM, only the detector is mounted on the mounting plate. The pressure transmitter must be ordered separately.

Unit：mm

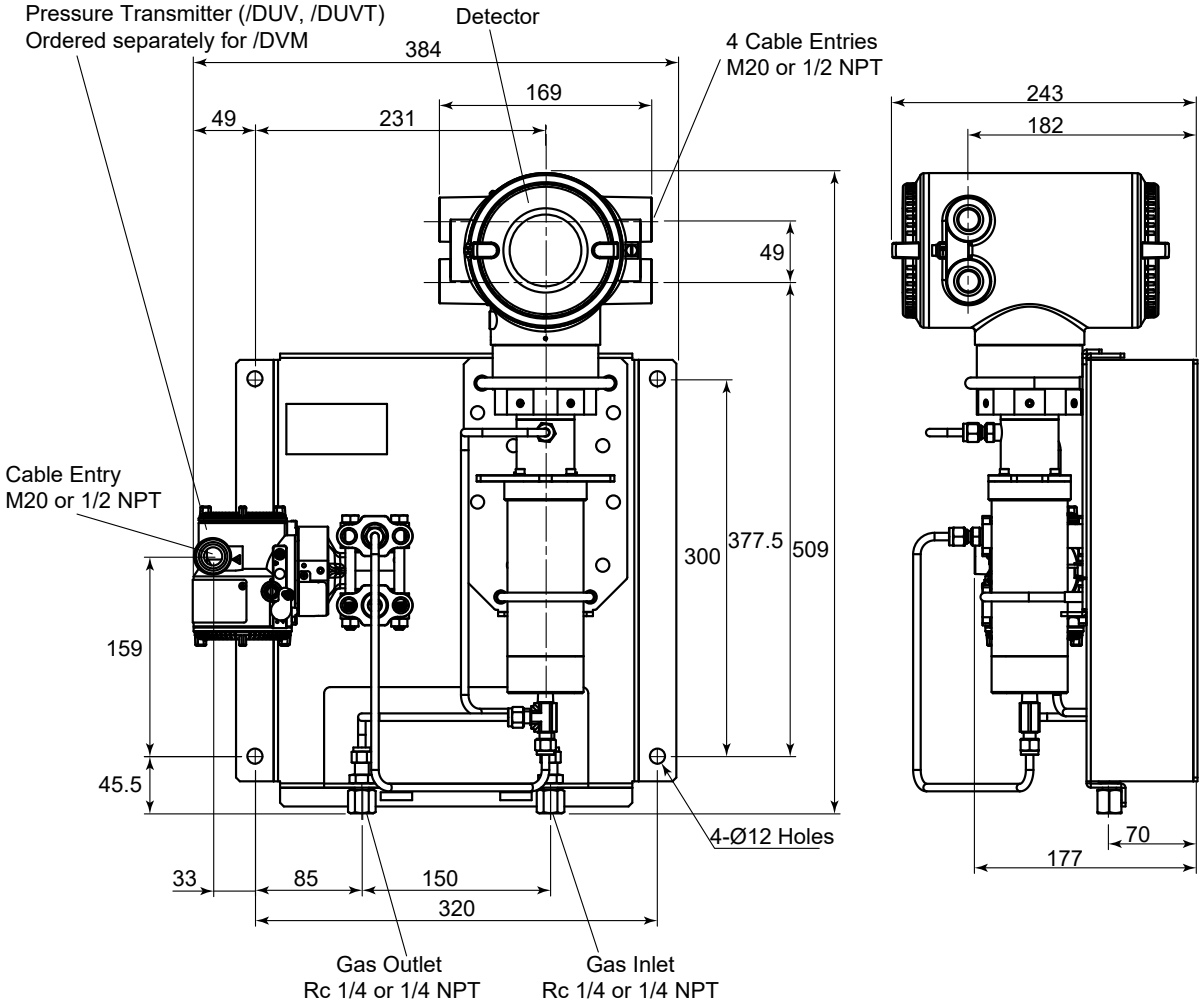

Note: Install the detector at a location capable of supporting the total weight of the detector mounted on the mounting plate (approx. 15.6 kg), cable glands, cables, and other associated components.

Weight: Approx. 15.6 kg (with mounting plate and EJX310A)

Unless otherwise specified, differences in the dimensions are specified as: General tolerance = ±(Criteria of tolerance class IT18 in JIS B0401-1998)/2.